

Sample Name :HA Peptide
Cat. No. : RP11735S
Lot. No. : 86337005122209ZW

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
Total Flow : 1 ml / min
Wavelength : 220 nm


Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
25.10	Pumps	Pump A B.Conc	95	
31.00	Pumps	Pump A B.Conc	95	
31.01	Pumps	Pump A B.Conc	5	
40.00	Pumps	Pump A B.Conc	5	
40.01	Controller	Stop		

<<Column Performance>>

<Detector A>

Column : AlltimaTM C18 4.6 x 250 mm

Chromatogram

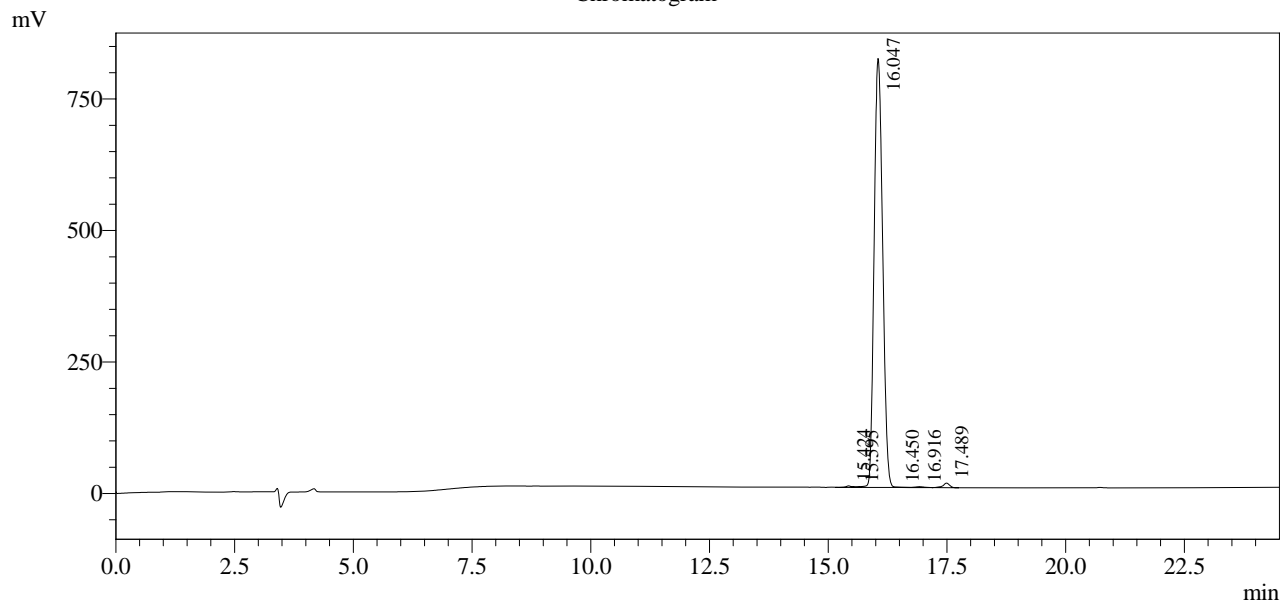

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	15.424	24441	2879	0.237
2	15.595	12250	1638	0.119
3	16.047	10170654	815637	98.528
4	16.450	8854	759	0.086
5	16.916	22211	1605	0.215
6	17.489	84179	8742	0.815
Total		10322589	831260	100.000