


Sample Name : SLLK, Control Peptide for TSP1 Inhibitor  
 Cat No. : RP19989

Pump A : 0.065% trifluoroacetic in 100% water  
 Pump A : 0.05% trifluoroacetic in 100% acetonitrile  
 TotalFlow: 1 ml/min  
 Wavelength: 214 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
30.00	Pumps	Pump A B.Conc	100	
42.00	Pumps	Pump A B.Conc	100	
43.00	Pumps	Pump A B.Conc	5	
49.00	Pumps	Pump A B.Conc	5	
50.00	Controller	Stop		

<Detector A>  
 Column : SHIMADZU VP-ODS 4.6 x 150 mm

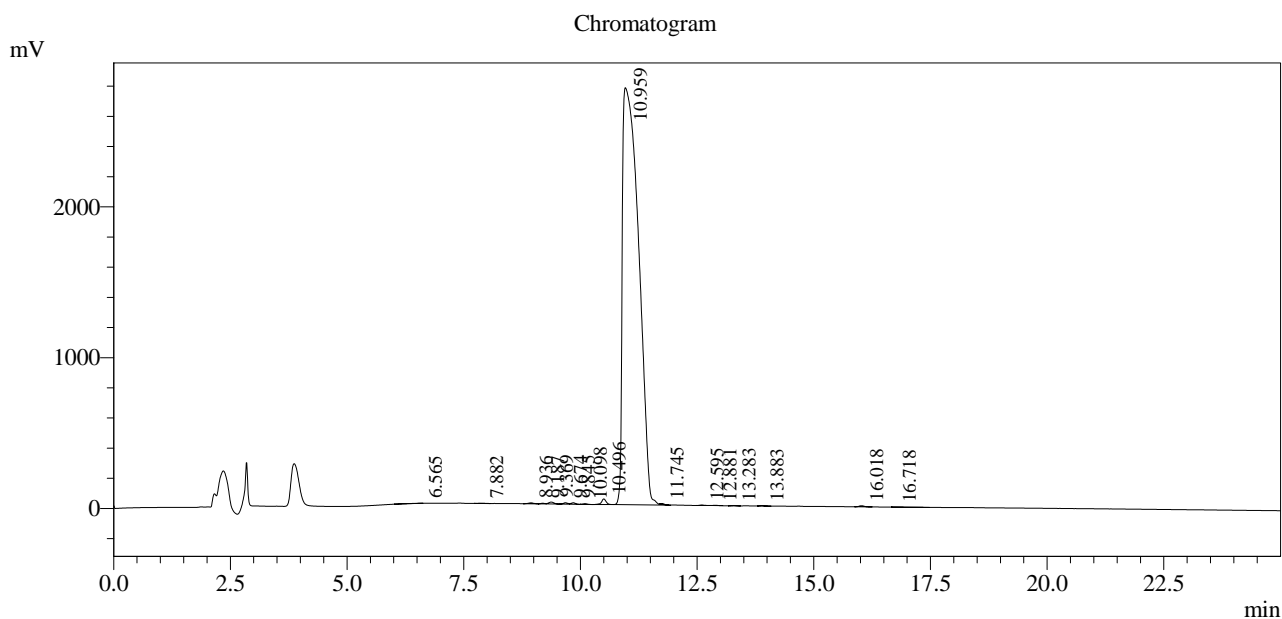

1 Det.A Ch1 / 214nm

Peak Table

Detector A Ch1 214nm

Peak#	Ret. Time	Area	Height	Area %
1	6.565	29358	600	0.044
2	7.882	14750	1538	0.022
3	8.936	46748	6102	0.069
4	9.187	23323	3956	0.035
5	9.369	93630	12360	0.139
6	9.674	59857	8811	0.089
7	9.845	61426	9345	0.091
8	10.098	28743	4646	0.043
9	10.496	252434	37313	0.374
10	10.959	66692312	2764918	98.868
11	11.745	25630	5117	0.038
12	12.595	17528	2719	0.026
13	12.881	13109	2012	0.019
14	13.283	12301	1941	0.018
15	13.883	16669	2669	0.025
16	16.018	55569	7398	0.082
17	16.718	12365	272	0.018
Total		67455751	2871717	100.000