


Positive MS Spectrum

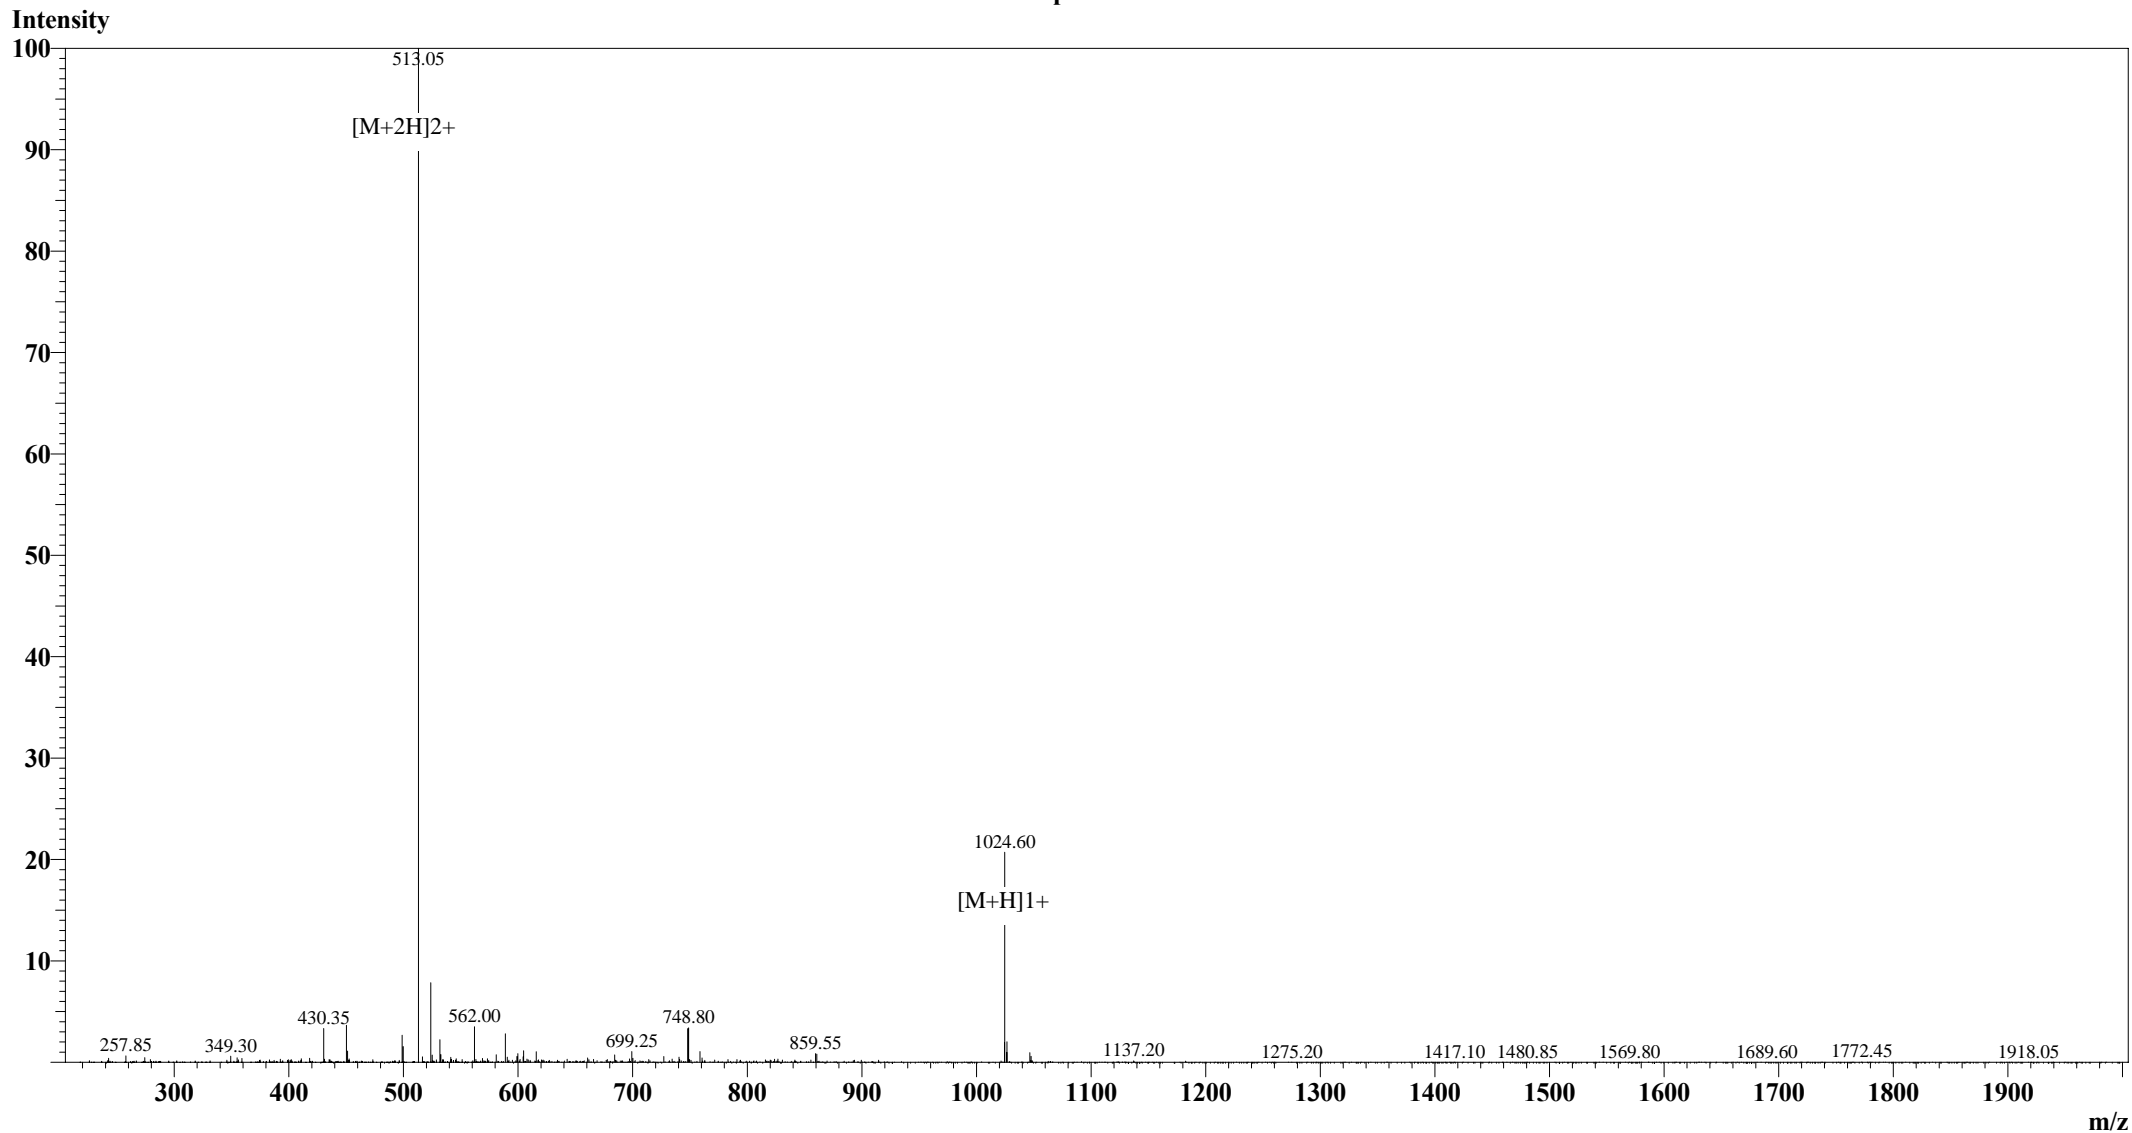

Sample Information

User : Grace
Date Acquired : 09/26/2009 11:34:58
Sample Name : Melanotan (MT)-II
Cat No. : RP17323
Lot No. : CE02909
Injection Volum : 1.000µL
Theoretical MW : 1024.18
Observed MW : 1023.60

Interface : ESI
Nebulizing Gas Flow : 1.50 L/min
CDL Temp : 250°C
CDL Volt : -25.0V
Block Temp : 200°C

Prerod Bias : +4.5kv
Detector : 1.5kv
T.Flow : 0.2ml/min
B.conc : 50%H2O/50%MeOH