


Mass Spectrum

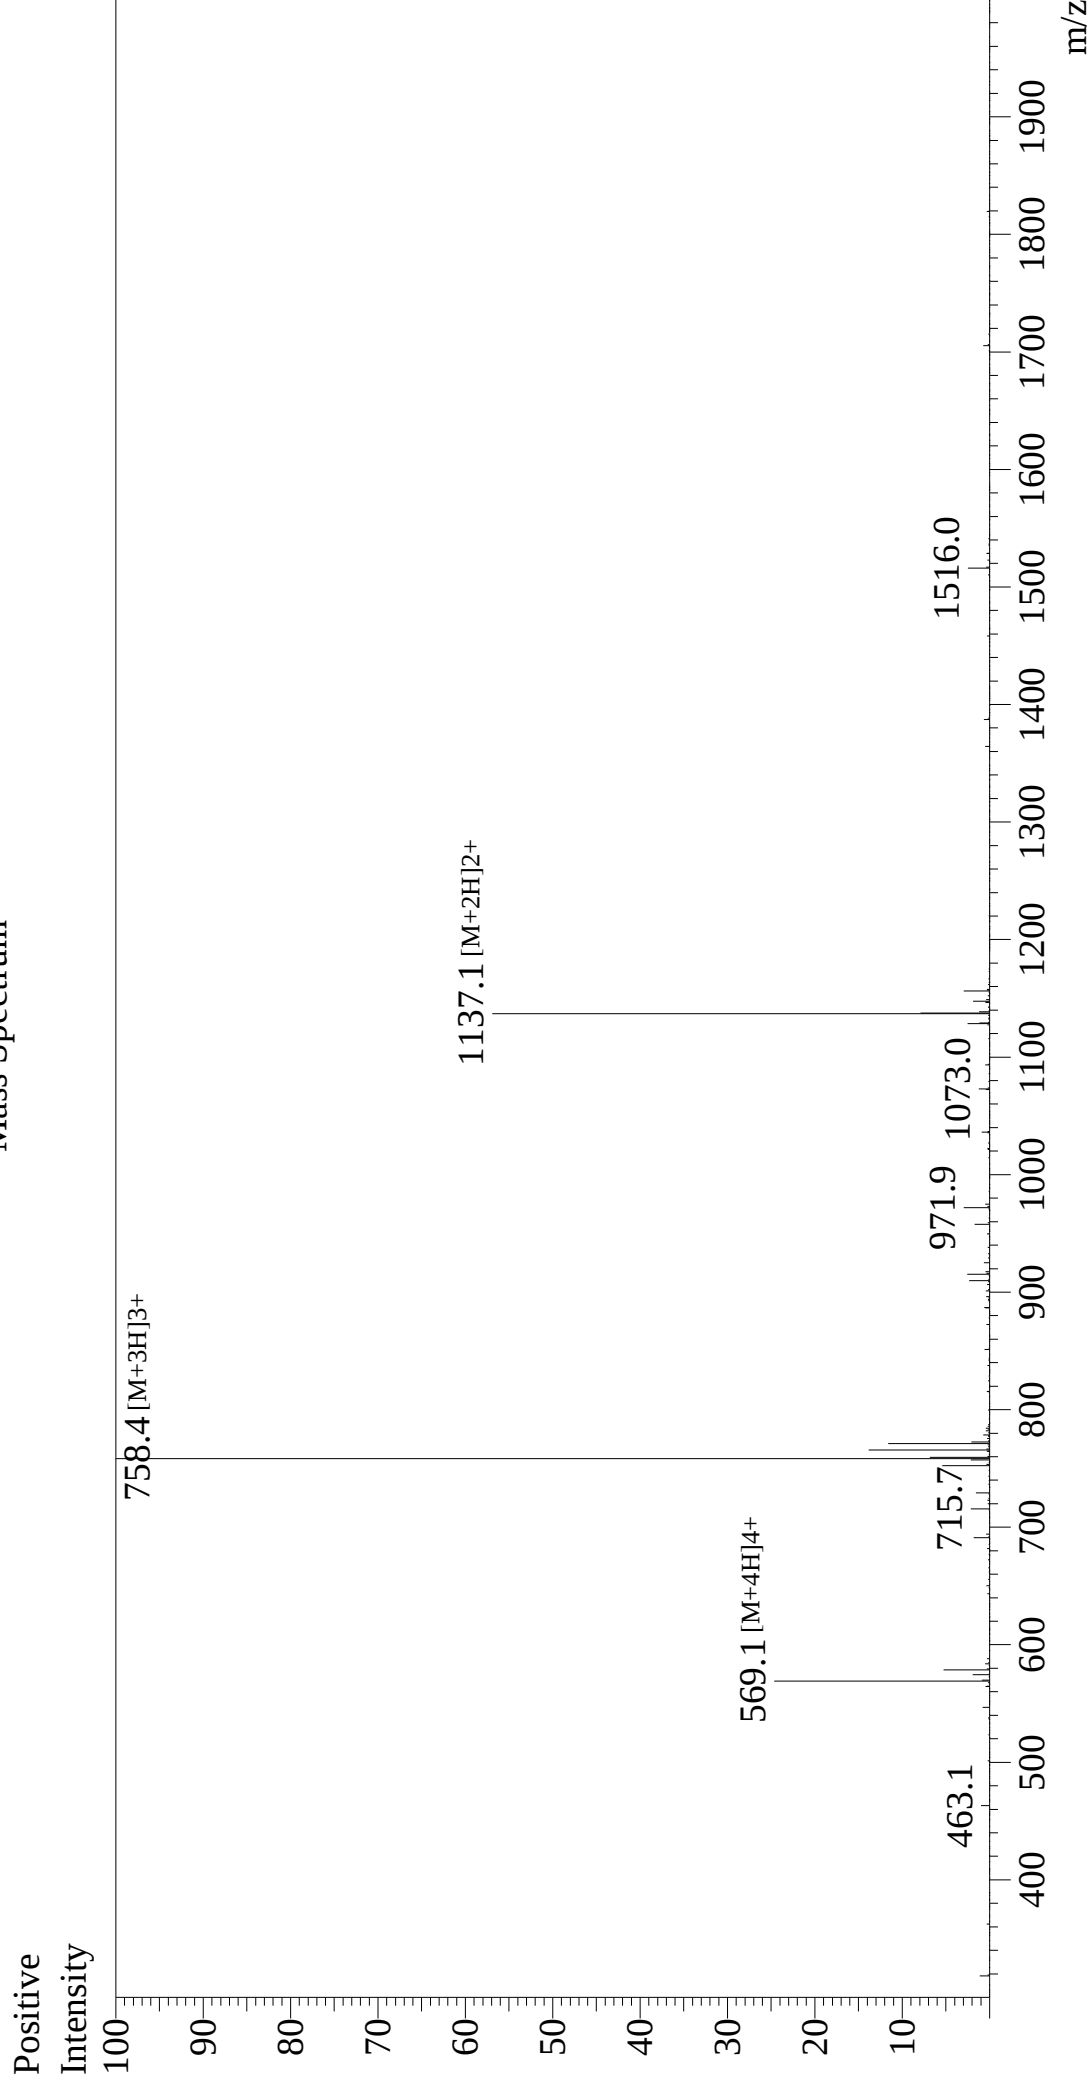

Sample Information

Month-Day Processed : 08/12/25
Time Processed : 20:49:58
Injection Volume : 0.5
Sample Name : Flagelin22
Cat No. : RP19986
Lot No. : E1231925H
Theoretical MW: 2272.50
Observed MW : 2272.2

Interface :ESI

Nebulizing Gas Flow :1.5L/min
CDL Temp :250
Block Temp :200

Equipment

: ZJ21010035
Interface Bias :+4.5 kV
Drying Gas Flow :5 L/min
T.Flow :0.2 ml/min
B.conc :50%H₂O/50%MeOH