


Mass Spectrum

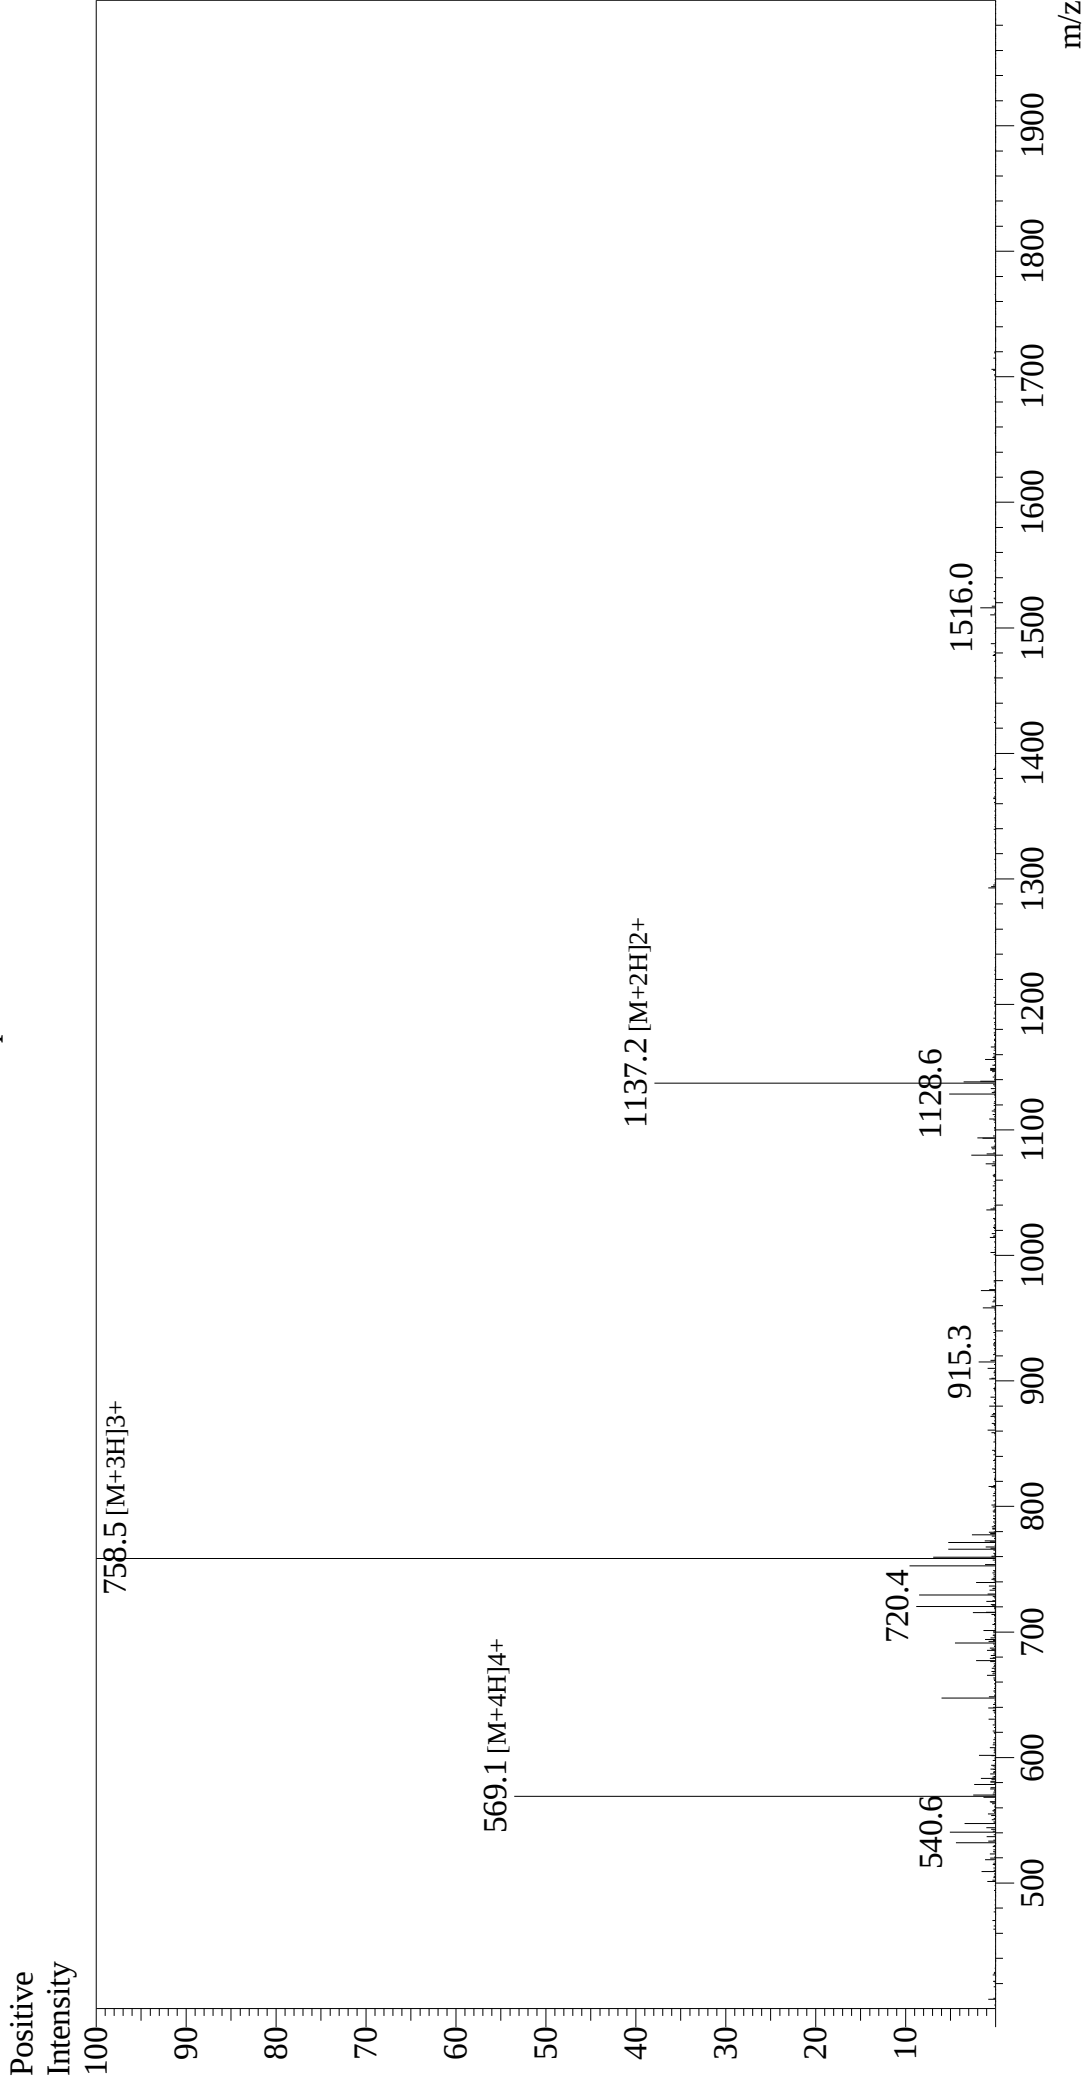

Sample Information

Month-Day Processed :	12/09/25	Equipment	:ZJ22010150
Time Processed :	14:25:34	Interface Bias	: +4.5 kV
Injection Volume :	0.2	Drying Gas Flow	:5 L/min
Sample Name :	Flagelin22	T.Flow	:0.2 ml/min
Cat No. : RP19986		B.conc	:50%H2O/50%MeOH
Lot No. : E1747925L			
Theoretical MW: 2272.50			
Observed MW : 2272.5			