

Sample Name:KRAS G12D Peptide (VVVGADGVGK)

Cat No. : RP30227

Lot No. : E1973224A

Time Processed :4:41:31 PM

Month-Day-Year Processed :01/18/2024

Pump A : 0.065% trifluoroacetic in 100% water (v/v)

Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)

Total Flow:1 ml/min

Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	B.Conc	5
25.00	Pumps	B.Conc	65
25.01	Pumps	B.Conc	95
27.00	Pumps	B.Conc	95
27.01	Pumps	B.Conc	5
35.00	Pumps	B.Conc	5
35.01	Controller	Stop	

<<Column Performance>>


<Detector A>

Column :Inertsil ODS-3 4.6 x 250 mm

Equipment: ZJ23010113

<Chromatogram>

mV

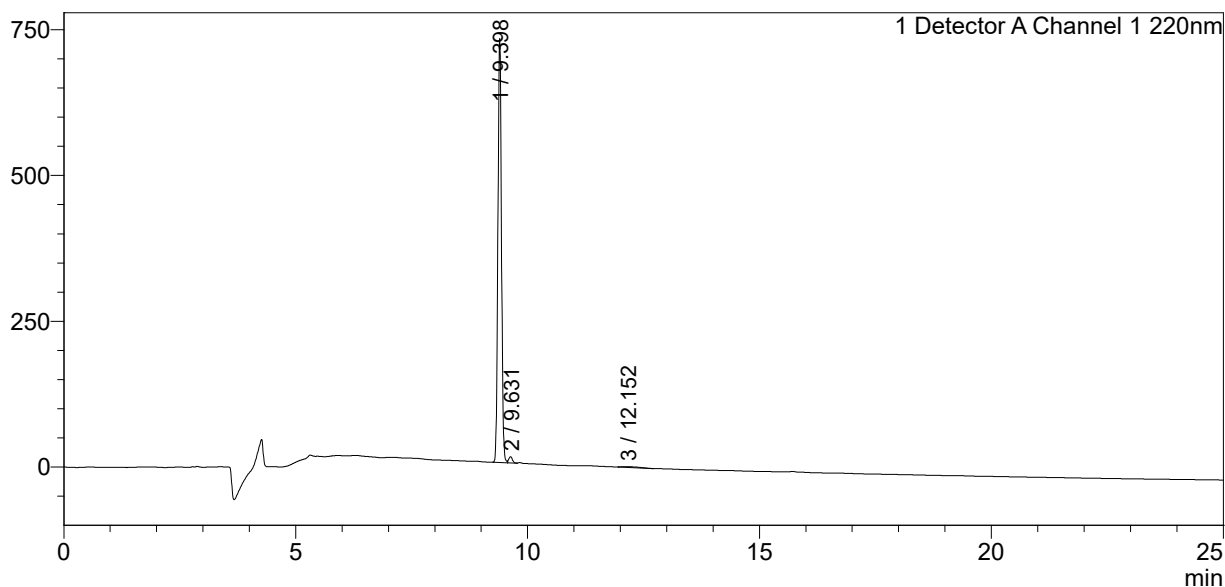

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	9.398	3887249	721378	97.848
2	9.631	55436	10597	1.395
3	12.152	30073	1095	0.757
Total		3972758	733071	100.000