


Mass Spectrum

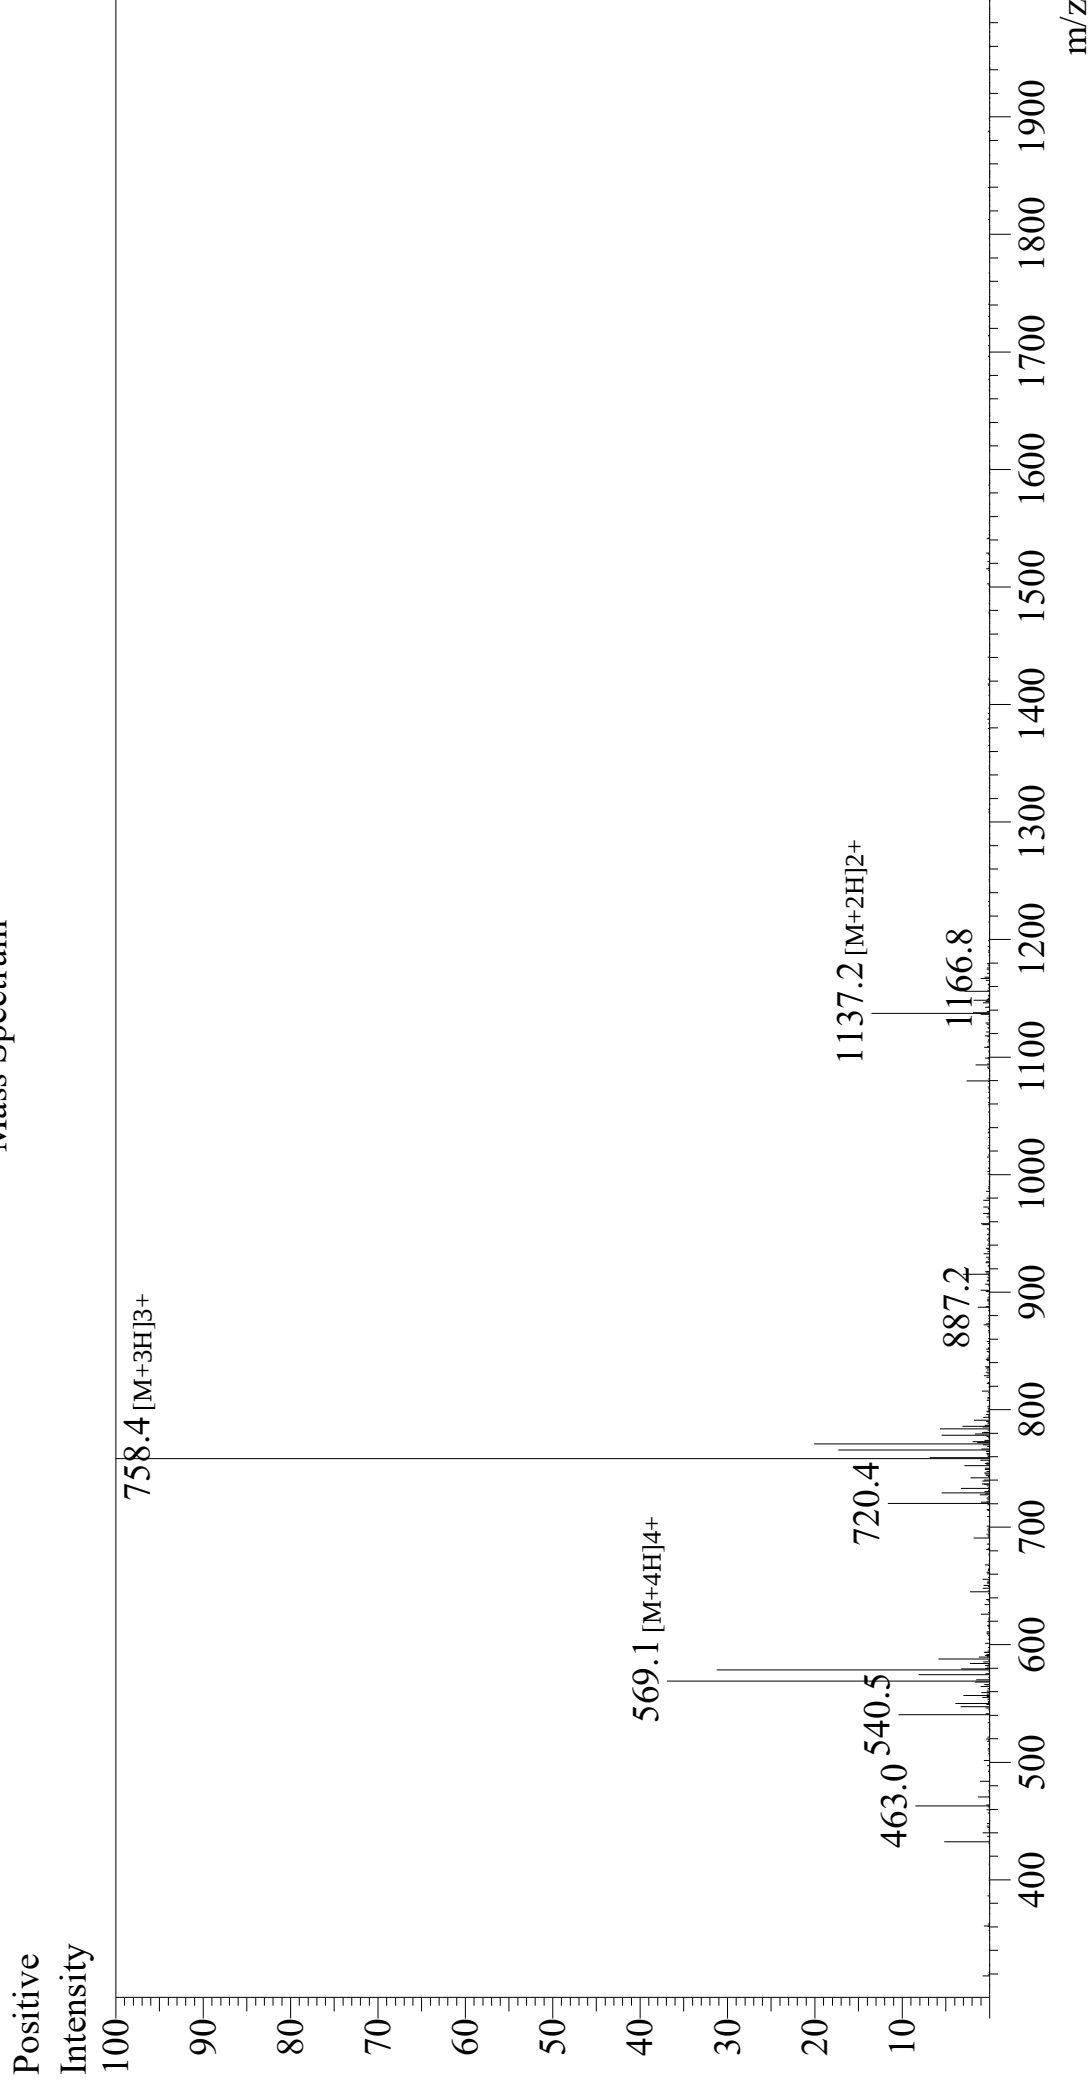

Sample Information

Month-Day Processed : 06/16/26
 Time Processed : 13:14:59
 Injection Volume : 0.4
 Sample Name : Flagelin22

Cat No. : RP19986

Lot No. : E2562226F

Theoretical MW: 2272.50

Observed MW : 2272.2

Interface : ESI

Nebulizing Gas Flow : 1.5L/min
 CDL Temp : 250
 Block Temp : 200

Equipment

Interface Bias : +4.5 kV
 Drying Gas Flow : 5 L/min
 T.Flow : 0.2 ml/min
 B.conc : 50% H₂O / 50% MeOH