


Mass Spectrum

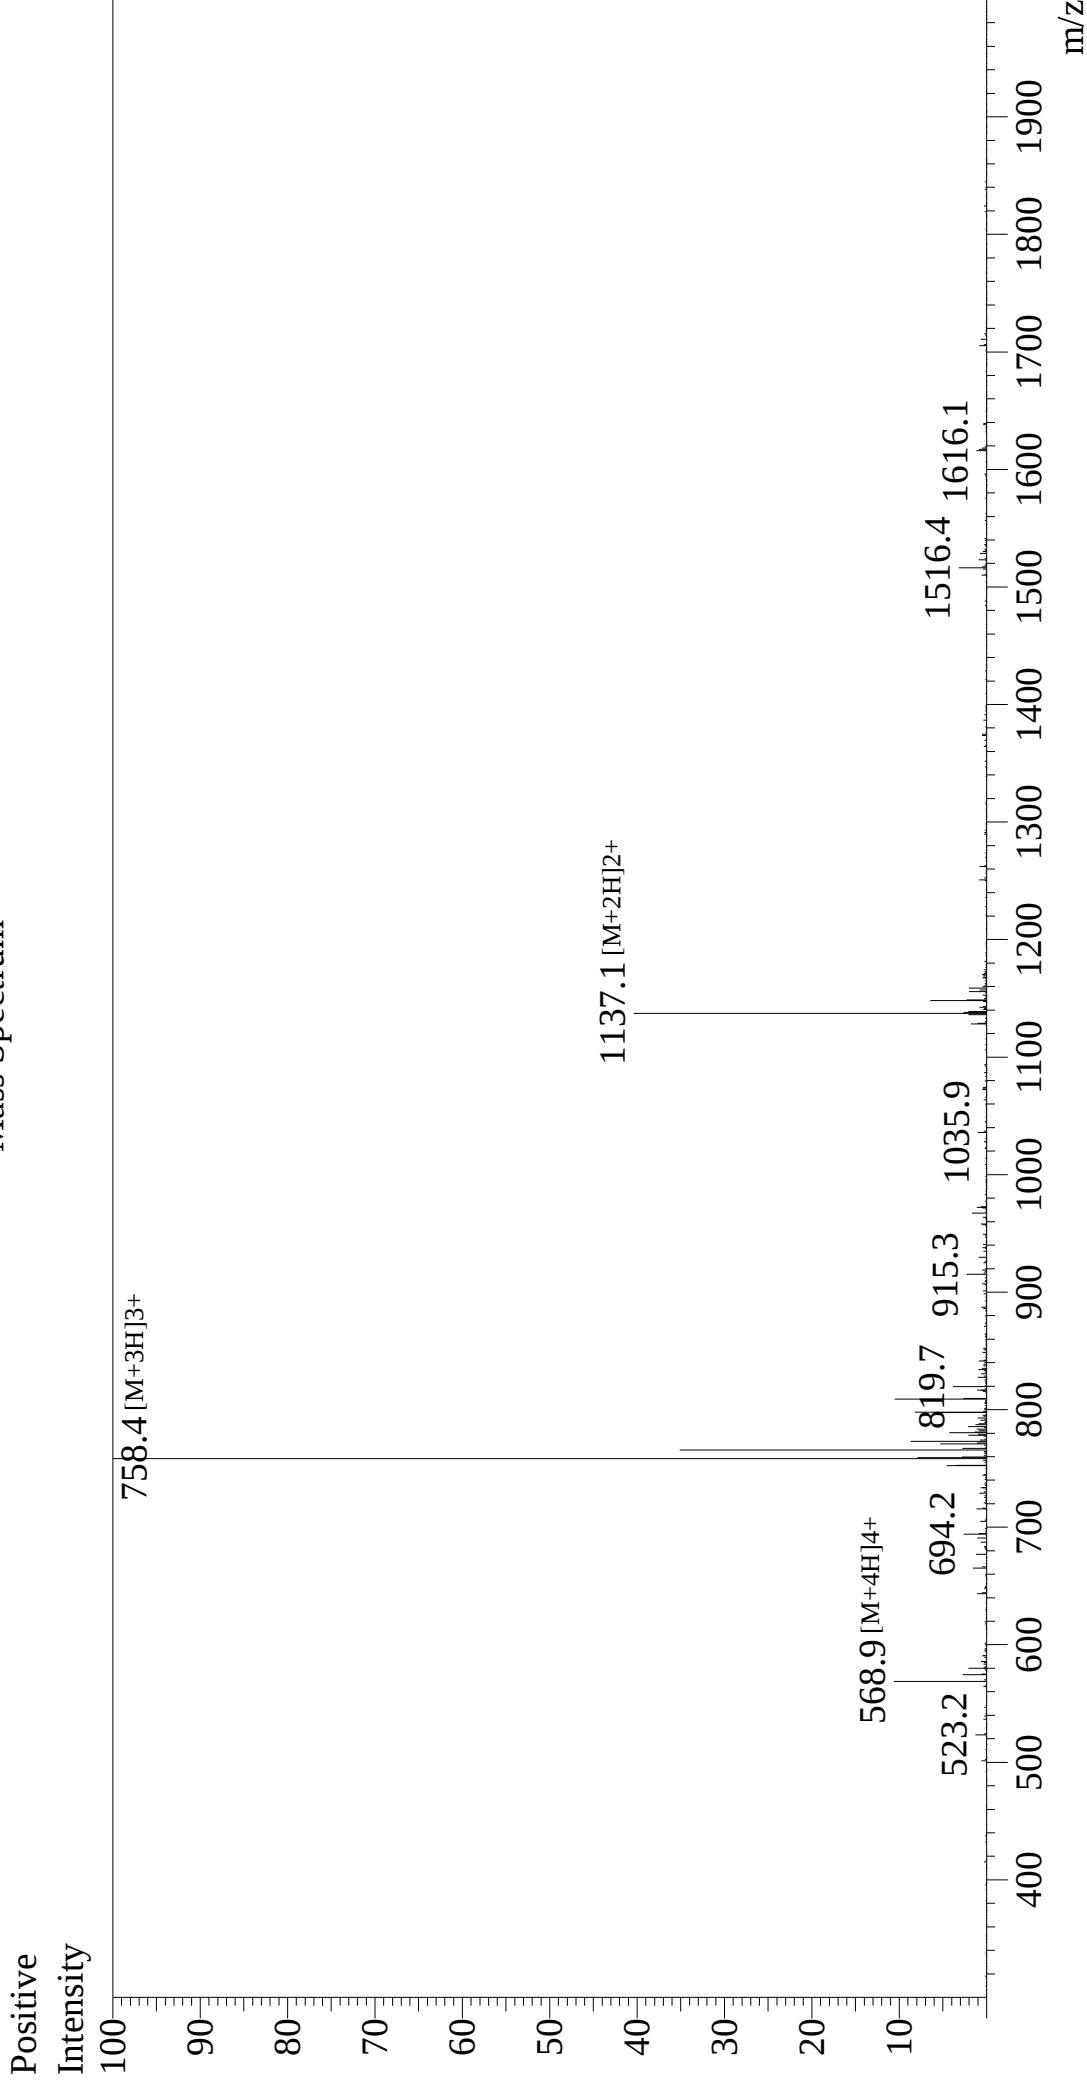

Sample Information

Month-Day Processed : 10/30/25
 Time Processed : 18:56:46
 Injection Volume : 0.3
 Sample Name : Flagelin22
 Cat No. : RP19986
 Lot No. : E3092225J
 Theoretical MW : 2272.50
 Observed MW : 2272.2

Interface

:ESI
 Nebulizing Gas Flow : 1.5L/min
 CDL Temp : 250
 Block Temp : 200

Equipment

: ZJ21010035
 Interface Bias : +4.5 kV
 Drying Gas Flow : 5 L/min
 T.Flow : 0.2 ml/min
 B.conc : 50%H2O/50%MeOH