


Mass Spectrum

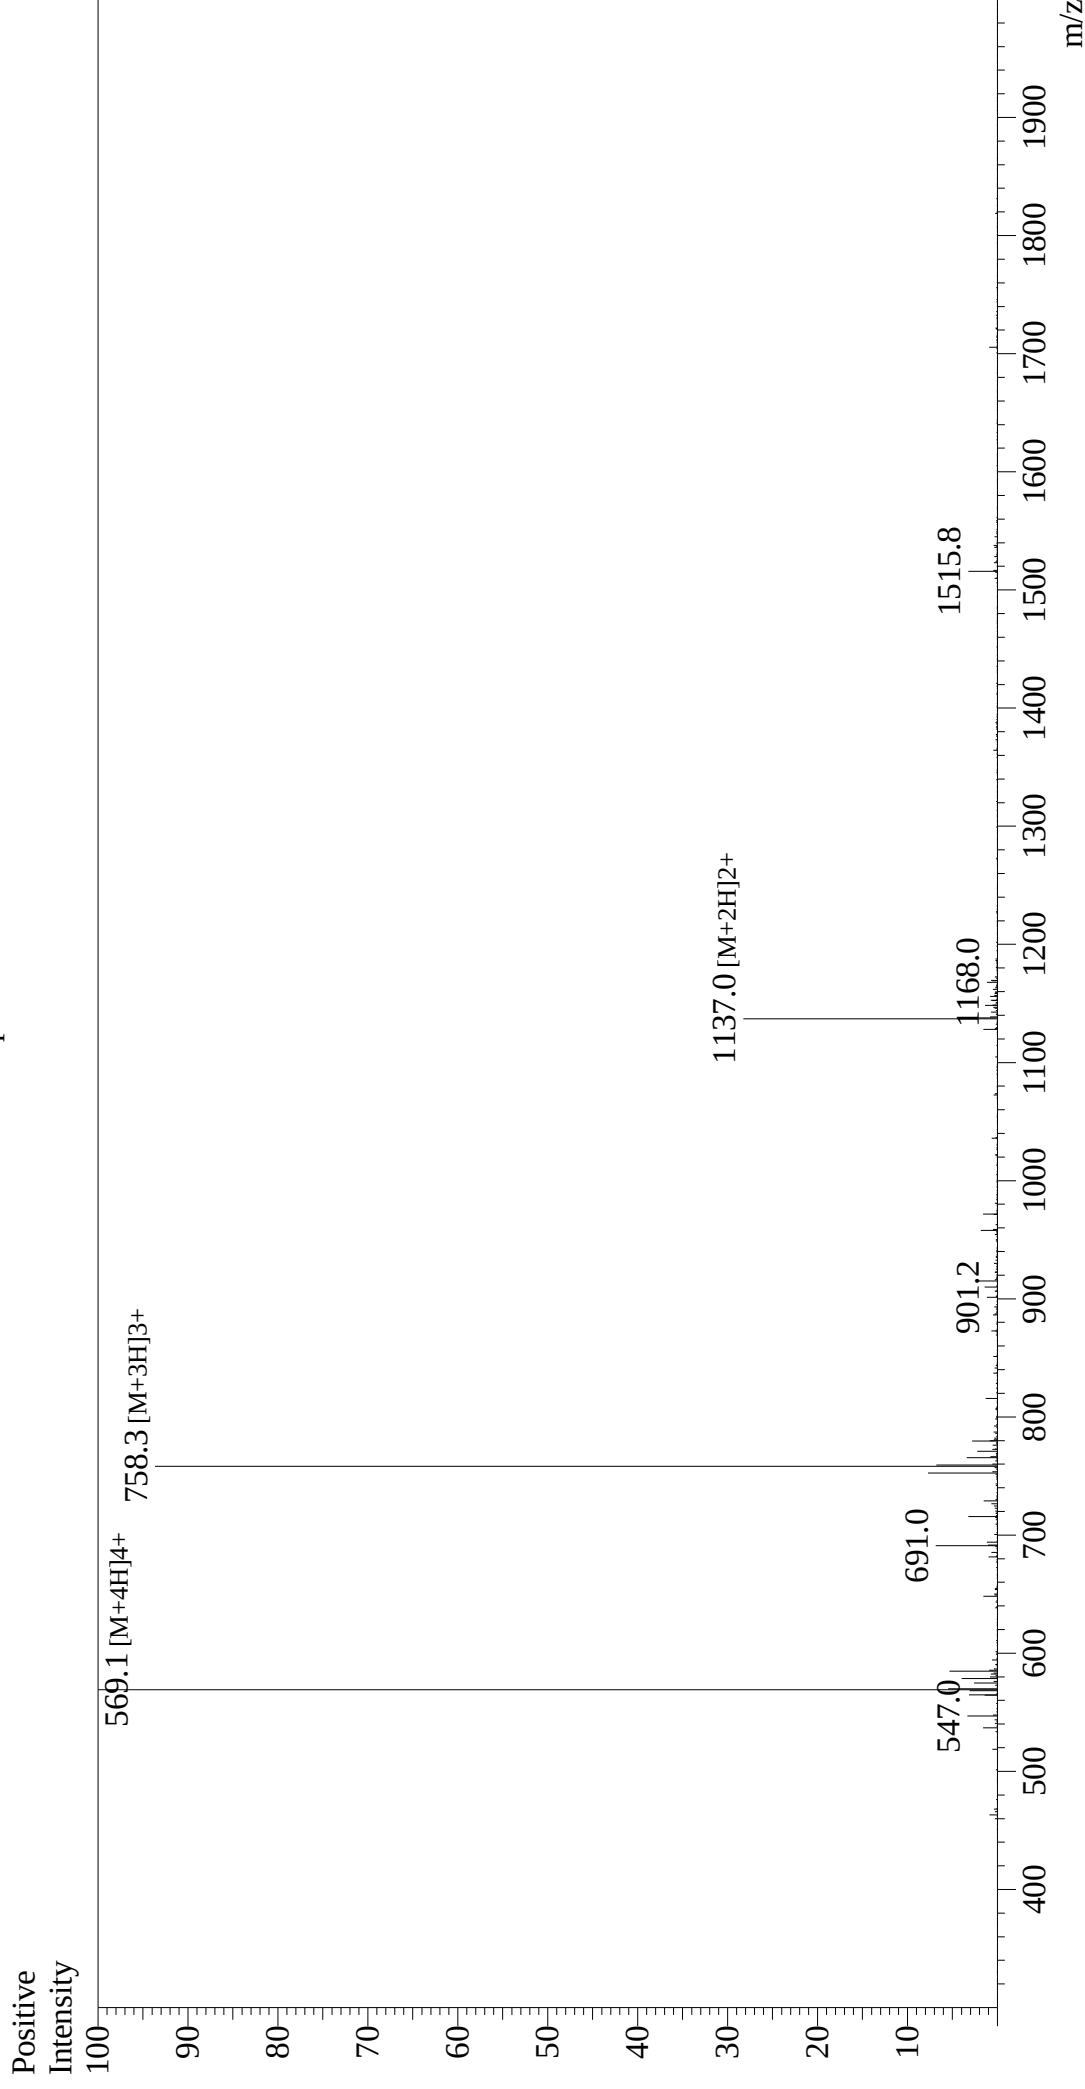

Sample Information

Month-Day Processed : 09/17/25
Time Processed : 3:52:47 PM
Injection Volume : 0.3
Sample Name : Flagelin22

Cat No. : RP19986
Lot No. : E3222825I

Theoretical MW: 2272.50

Observed MW : 2272.4

Interface

Nebulizing Gas Flow :1.5L/min
CDL Temp :250
Block Temp :200

Equipment

: ZJ21010035
Interface Bias : +4.5 kV
Drying Gas Flow :5 L/min
T.Flow :0.2 ml/min
B.conc :50%H2O/50%MeOH