


Mass Spectrum

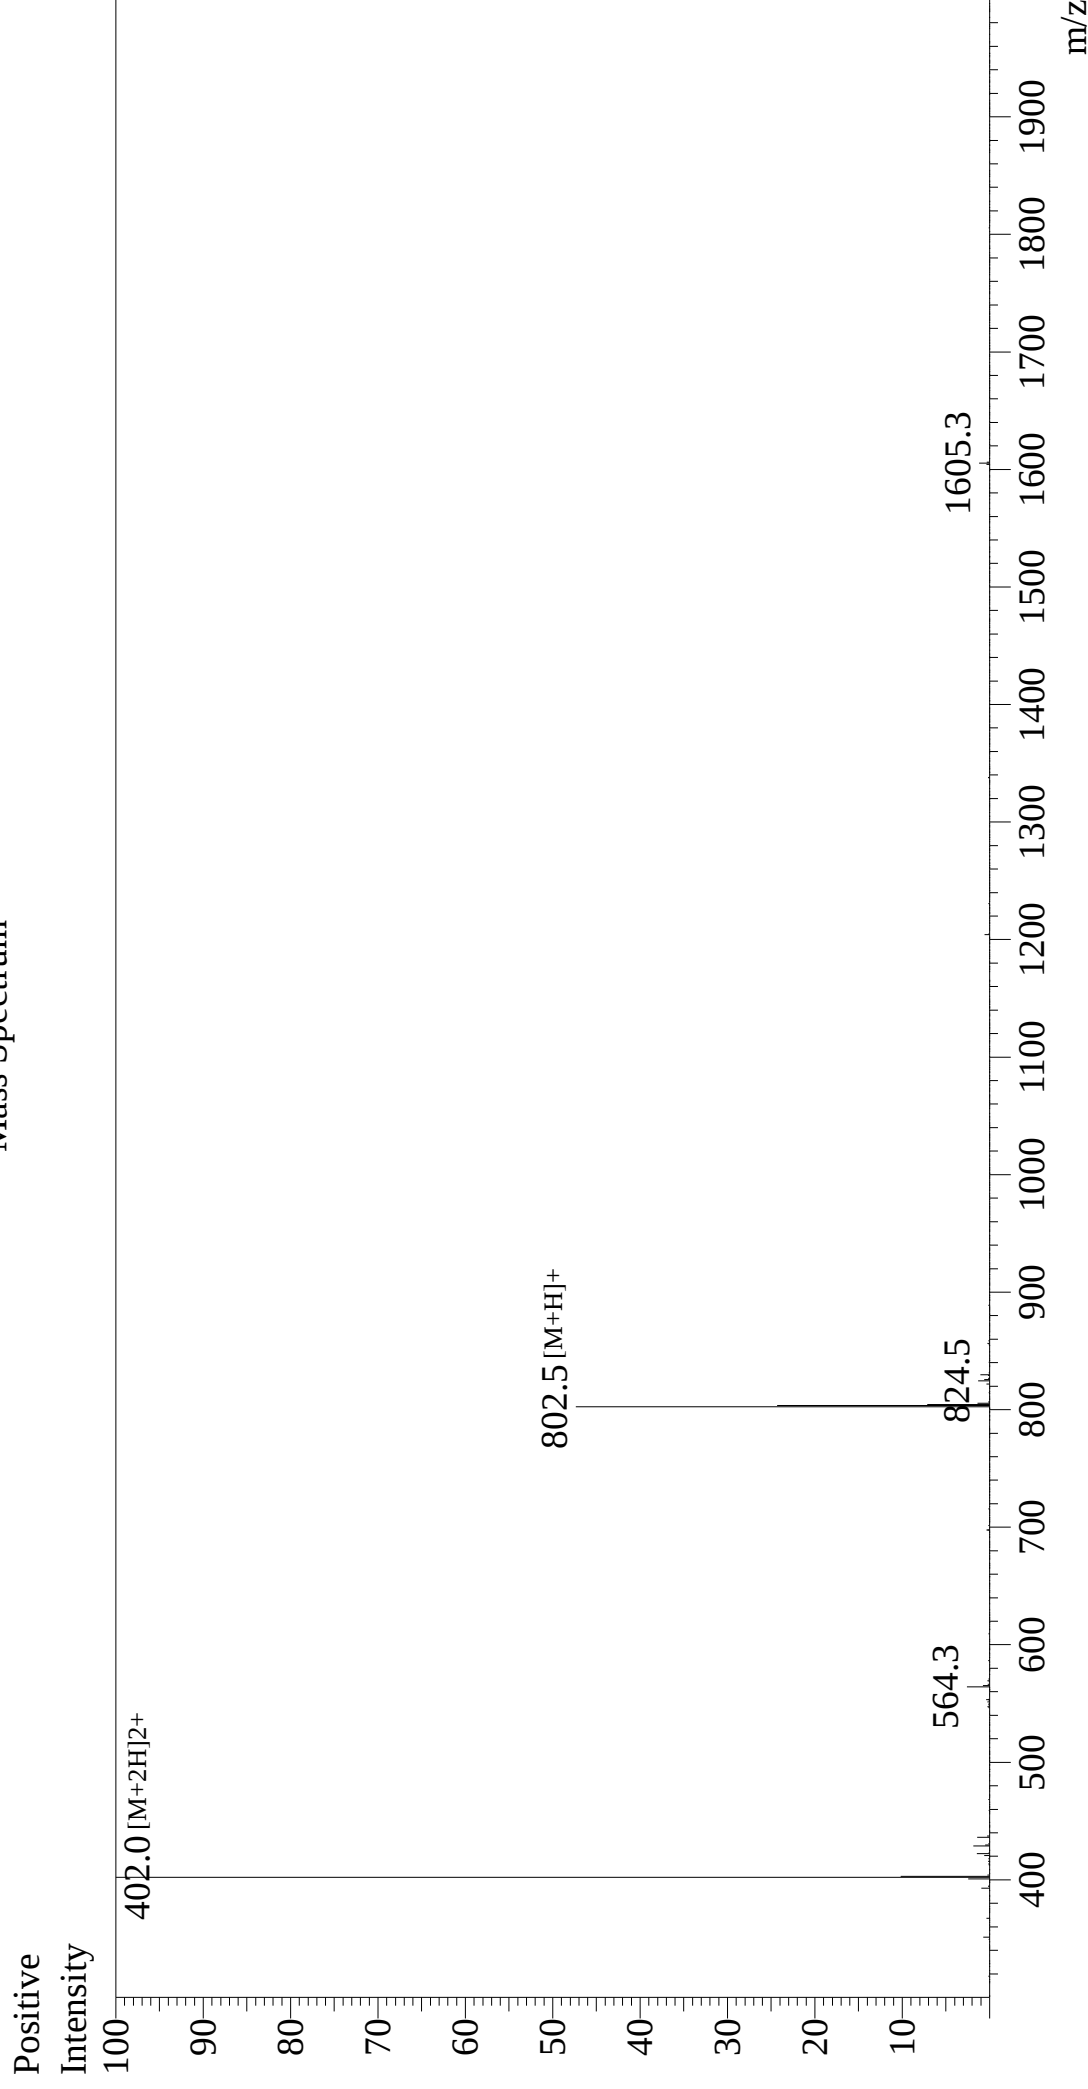

Sample Information

Month-Day Processed : 05/28/26
Time Processed : 8:41:14
Injection Volume : 0.3
Sample Name : GS-PepFirming™ Palmitoyl Pentapeptide-4
Cat No. : RP30039
Lot No. : E3327626E

Theoretical MW: 802.10
Observed MW : 802.0

Interface :ESI

Nebulizing Gas Flow :1.5L/min
CDL Temp :250
Block Temp :200

Equipment

: ZJ21010035
Interface Bias :+4.5 kV
Drying Gas Flow :5 L/min
T.Flow :0.2 ml/min
B.conc :50%H2O/50%MeOH