


Mass Spectrum

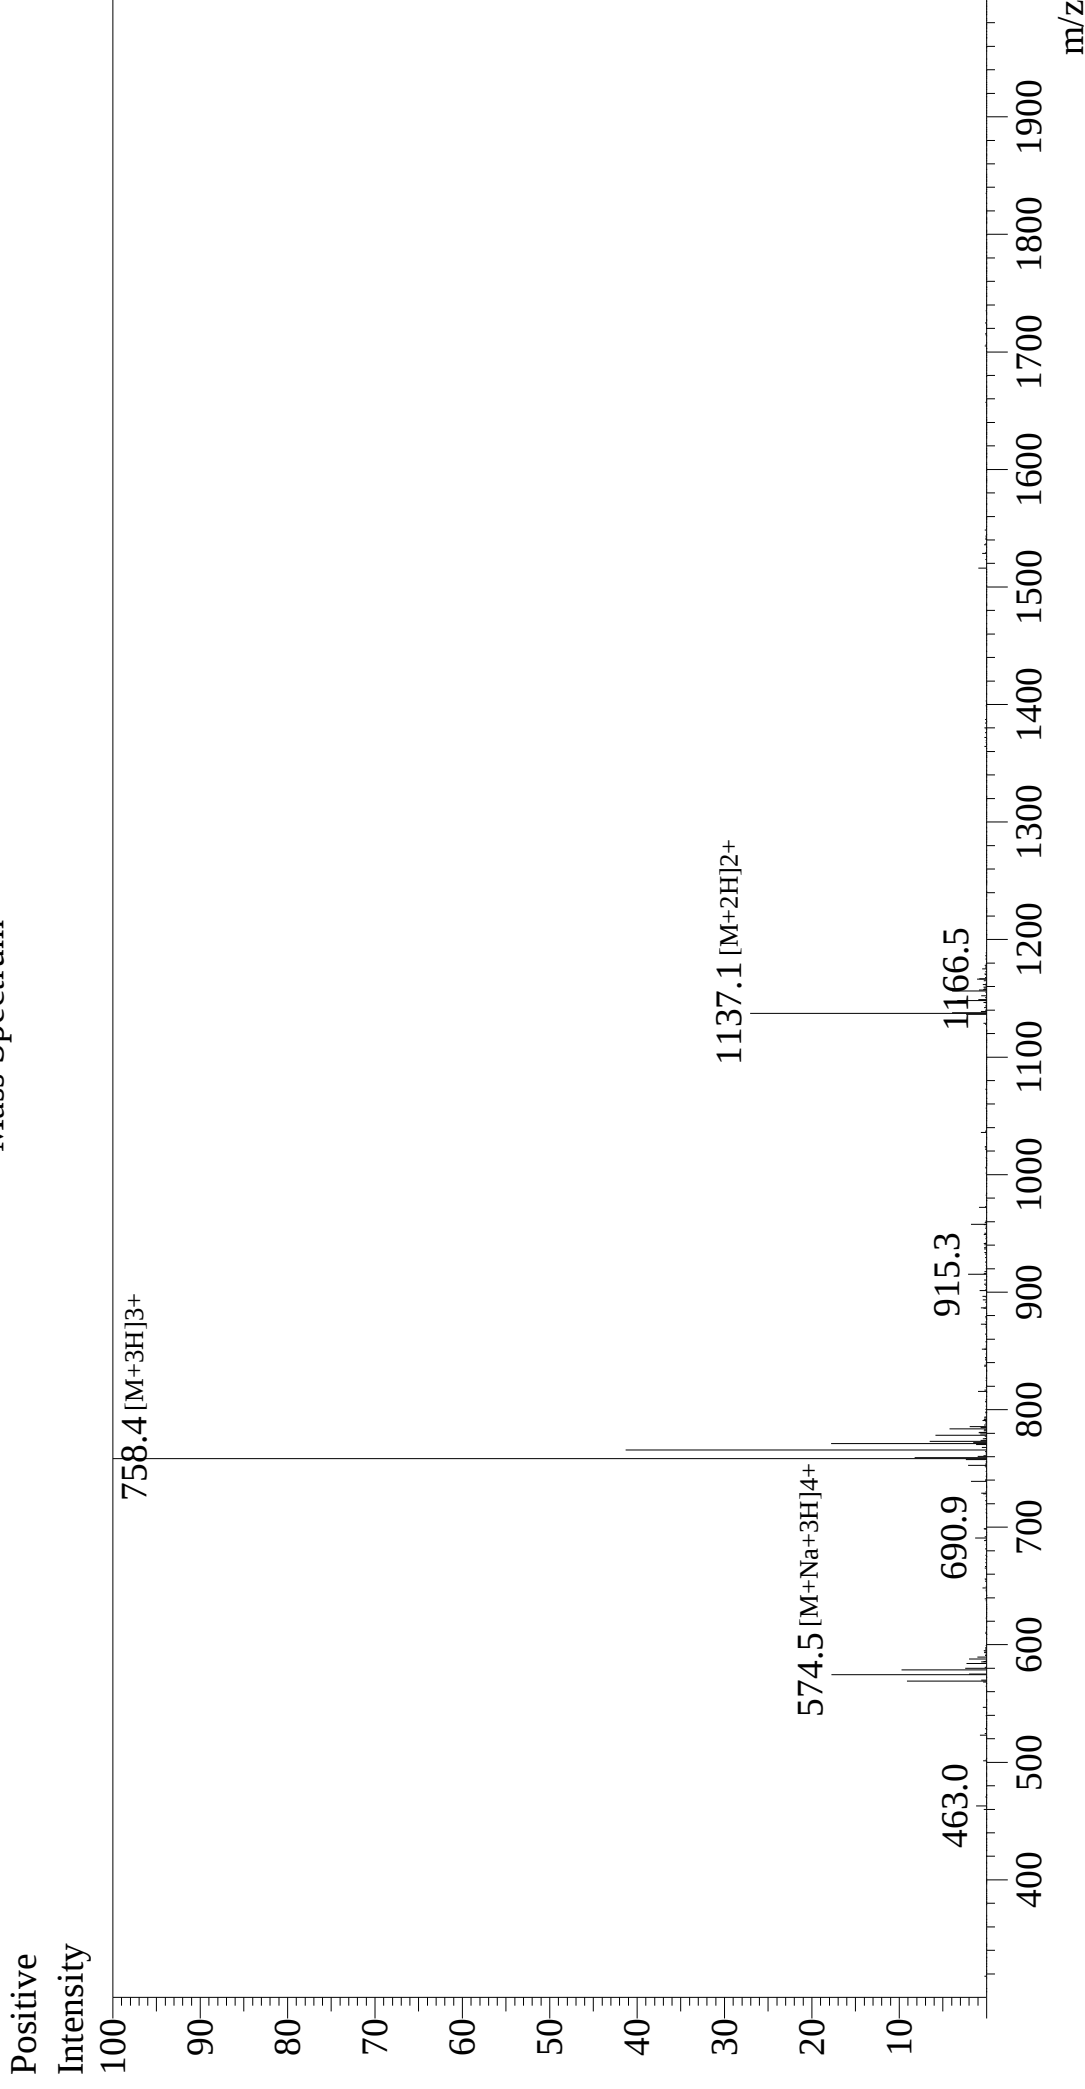

Sample Information

Month-Day Processed :	01/30/26	Equipment	: ZJ21010035
Time Processed :	9:19:45 AM	Interface	: ESI
Injection Volume :	0.4	Nebulizing Gas Flow	: 1.5L/min
Sample Name :	Flagelin22	CDL Temp	: 250
Cat No. : RP19986		Block Temp	: 200
Lot No. : E5886526A			
Theoretical MW: 2272.50			
Observed MW : 2272.2			
		Drying Gas Flow	: 5 L/min
		T.Flow	: 0.2 ml/min
		B.conc	: 50%H2O/50%MeOH