


Mass Spectrum

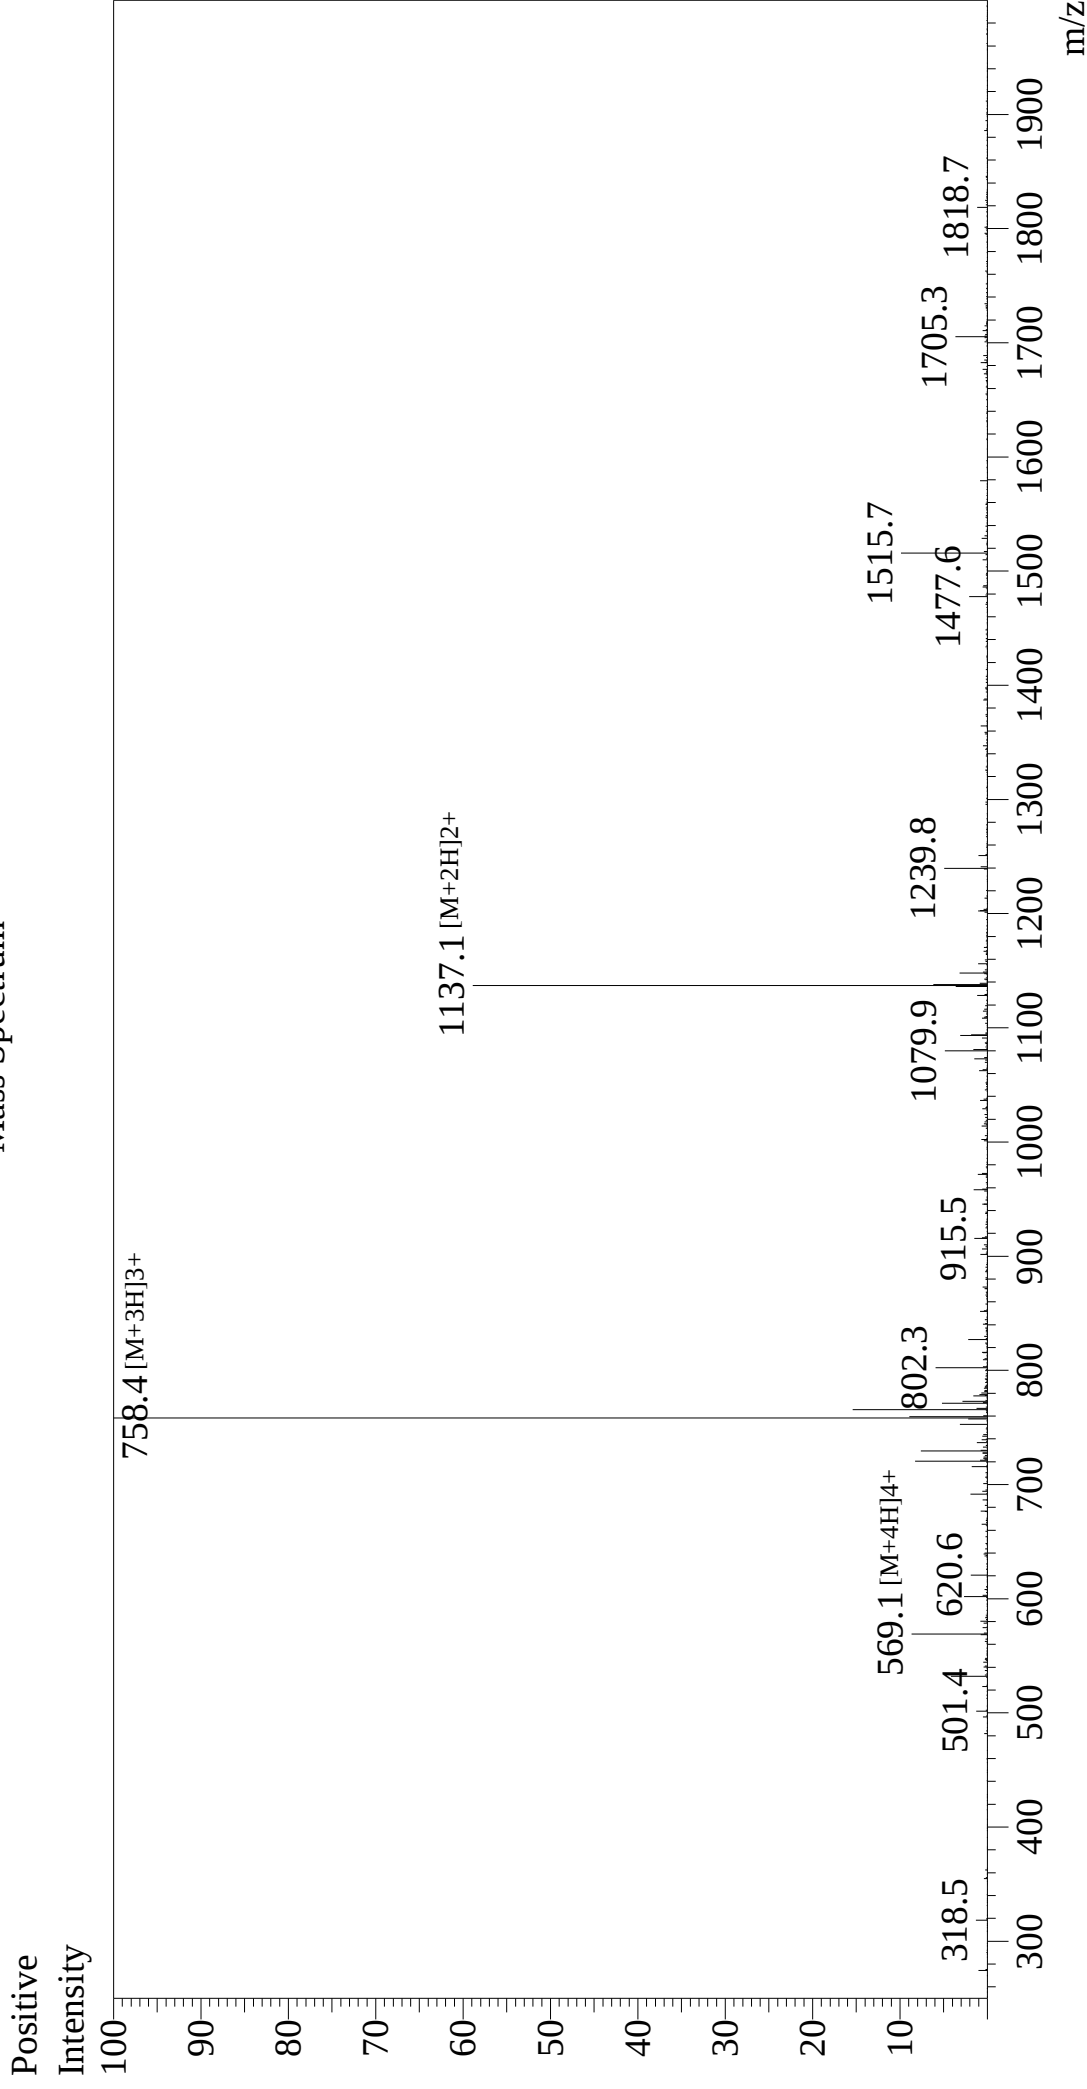

Sample Information

Month-Day Processed : 03/31/26
Time Processed : 22:34:20
Injection Volume : 0.3
Sample Name : Flagelin22
Cat No. : RP19986
Lot No. : E6823226C
Theoretical MW : 2272.50
Observed MW : 2272.2

Interface : ESI
Nebulizing Gas Flow : 1.5L/min
CDL Temp : 250
Block Temp : 200

Equipment
Interface Bias
Drying Gas Flow
T.Flow
B.conc

: ZJ22010150
: +4.5 kV
: 5 L/min
: 0.2 ml/min
: 50%H2O/50%MeOH