


Mass Spectrum

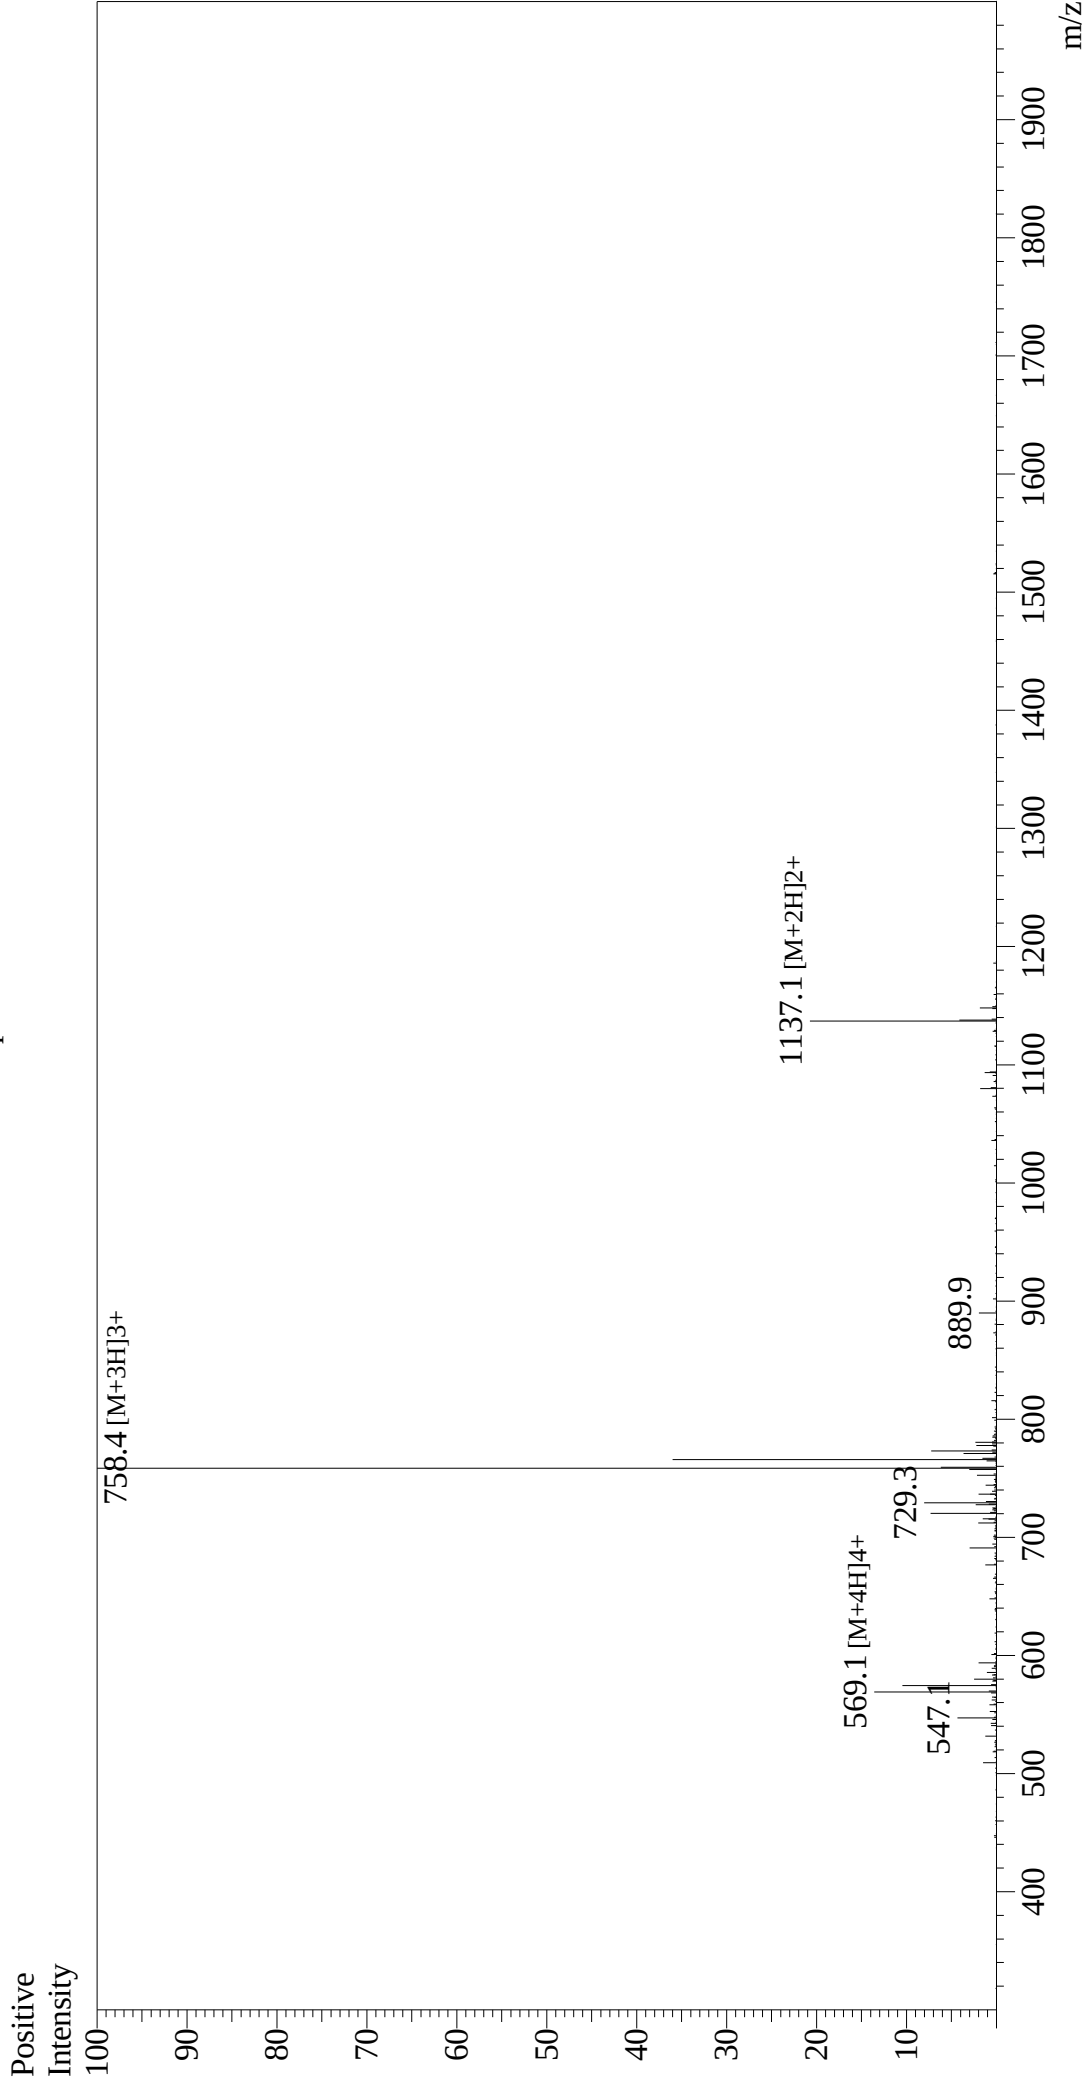

Sample Information

Month-Day Processed : 01/13/26

Time Processed : 20:17:03

Injection Volume : 0.4

Sample Name : Flagelin22

Cat No. : RP19986

Lot No. : E7182426A

Theoretical MW: 2272.50

Observed MW : 2272.2

Interface

Interface : ESI

Nebulizing Gas Flow : 1.5L/min

CDL Temp : 250

Block Temp : 200

Equipment

Equipment : ZJ21010035

Interface Bias : +4.5 kV

Drying Gas Flow : 5 L/min

T.Flow : 0.2 ml/min

B.conc : 50%H2O/50%MeOH