


# Mass Spectrum

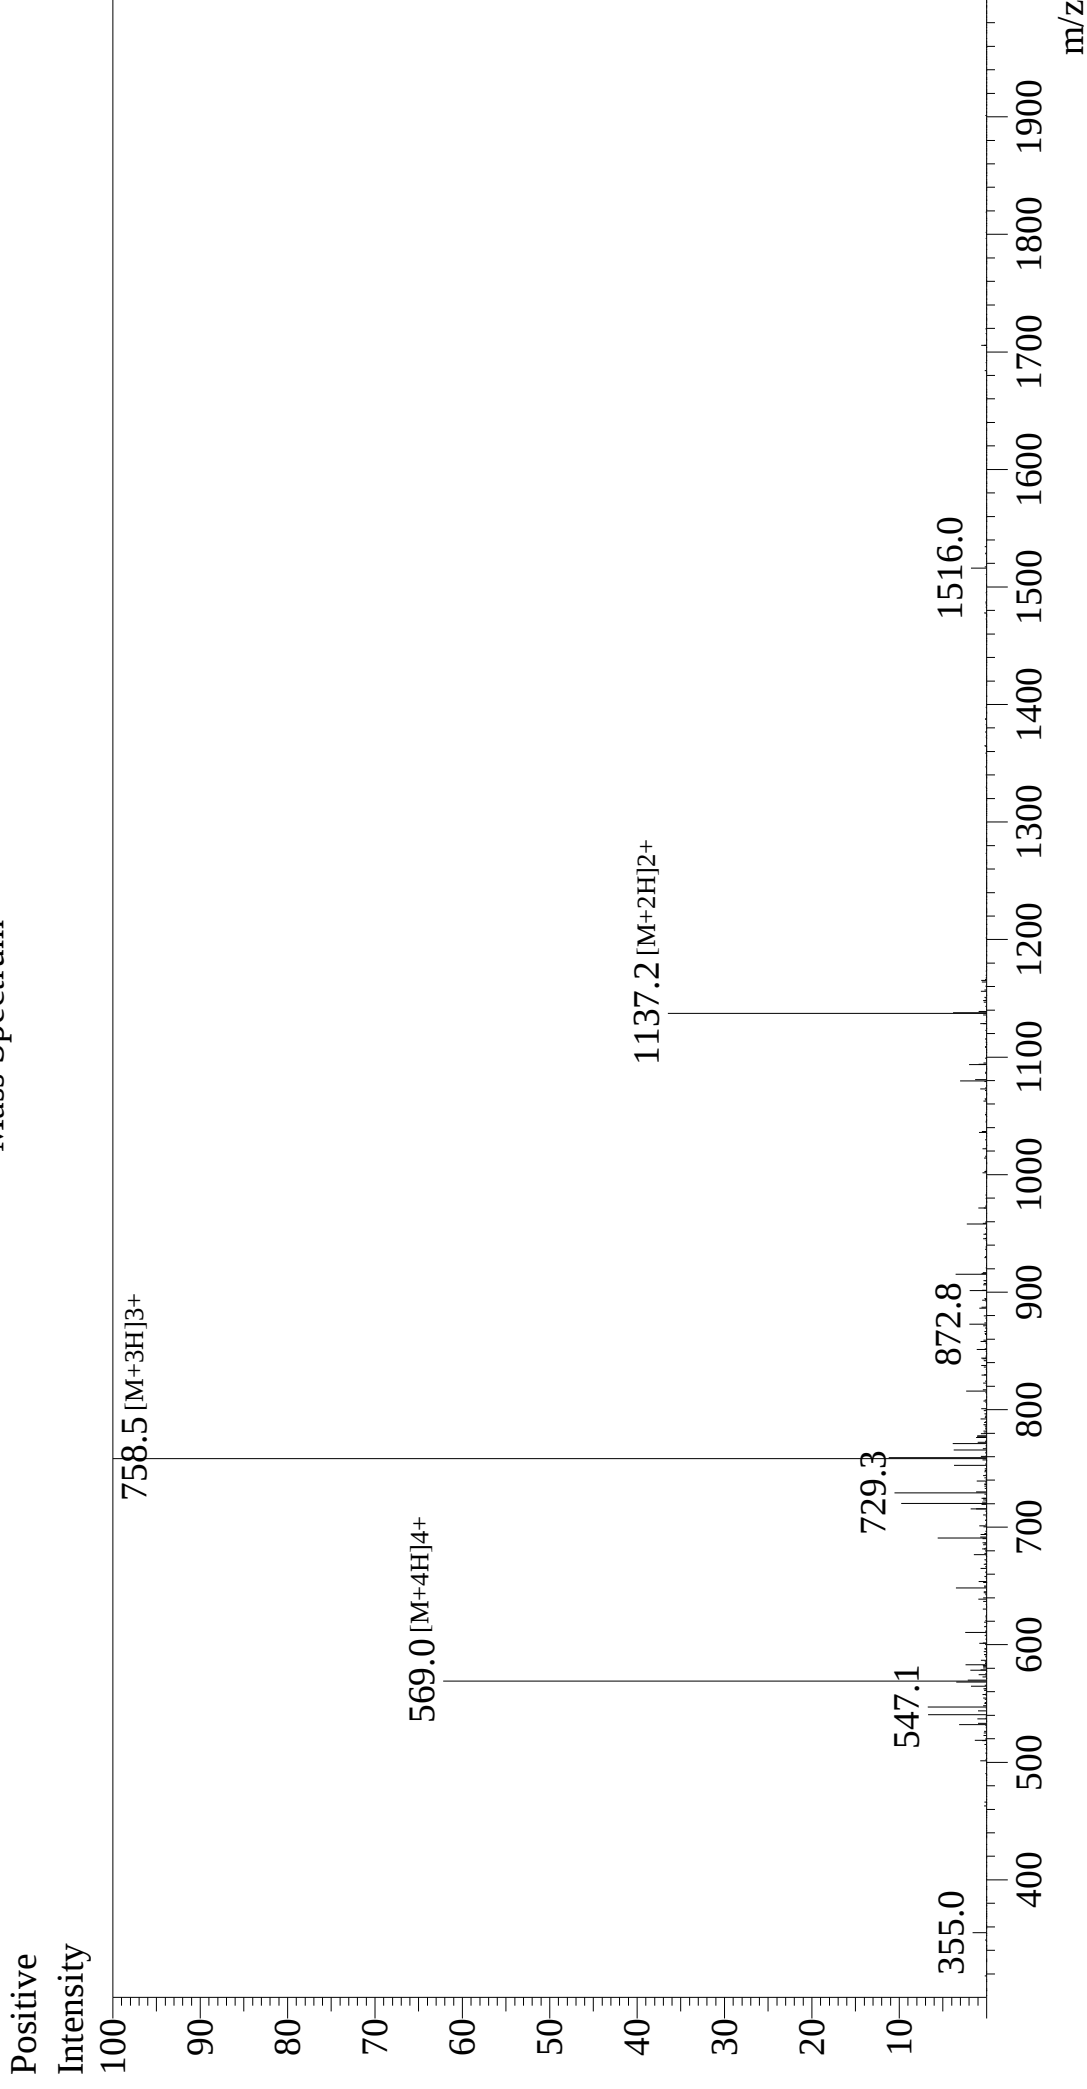

## Sample Information

Month-Day Processed : 05/08/26  
Time Processed : 9:27:50  
Injection Volume : 0.5  
Sample Name : Flagelin22  
Cat No. : RP19986  
Lot No. : E7688426E

Theoretical MW: 2272.51  
Observed MW : 2272.5

## Interface :ESI

Nebulizing Gas Flow :1.5L/min  
CDL Temp :250  
Block Temp :200

## Equipment

: ZJ21010035  
Interface Bias : +4.5 kV  
Drying Gas Flow :5 L/min  
T.Flow :0.2 ml/min  
B.conc :50%H<sub>2</sub>O/50%MeOH