

Sample Name: Humanin, HN
 Cat No. : RP30893
 Lot No. : E7749826A
 Time Processed : 3:16:53
 Month-Day-Year Processed : 01/30/2026

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow: 1 ml/min
 Wavelength: 220 nm

<<LC Time Program>>


Time	Module	Command	Value
0.01	Pumps	B.Conc	5
25.00	Pumps	B.Conc	65
25.01	Pumps	B.Conc	95
27.00	Pumps	B.Conc	95
27.01	Pumps	B.Conc	5
35.00	Pumps	B.Conc	5
35.01	Controller	Stop	

<<Column Performance>>

<Detector A>

Column : Inertsil ODS-SP 4.6 x 250 mm
 Equipment : ZJ20010140

<Chromatogram>

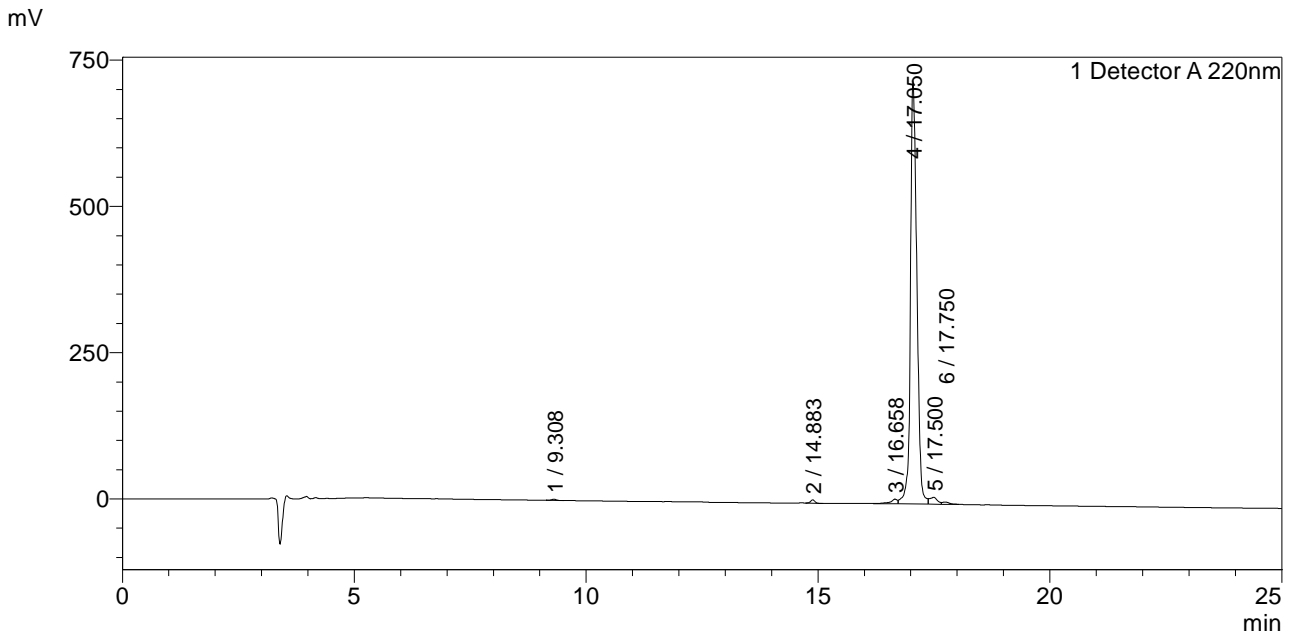

<Peak Table>

Detector A 220nm

Peak#	Ret. Time	Area	Height	Area%
1	9.308	13924	2112	0.192
2	14.883	39589	5919	0.546
3	16.658	87283	8139	1.204
4	17.050	6919763	719759	95.460
5	17.500	142483	11756	1.966
6	17.750	45828	3934	0.632
Total		7248871	751618	100.000