


Mass Spectrum

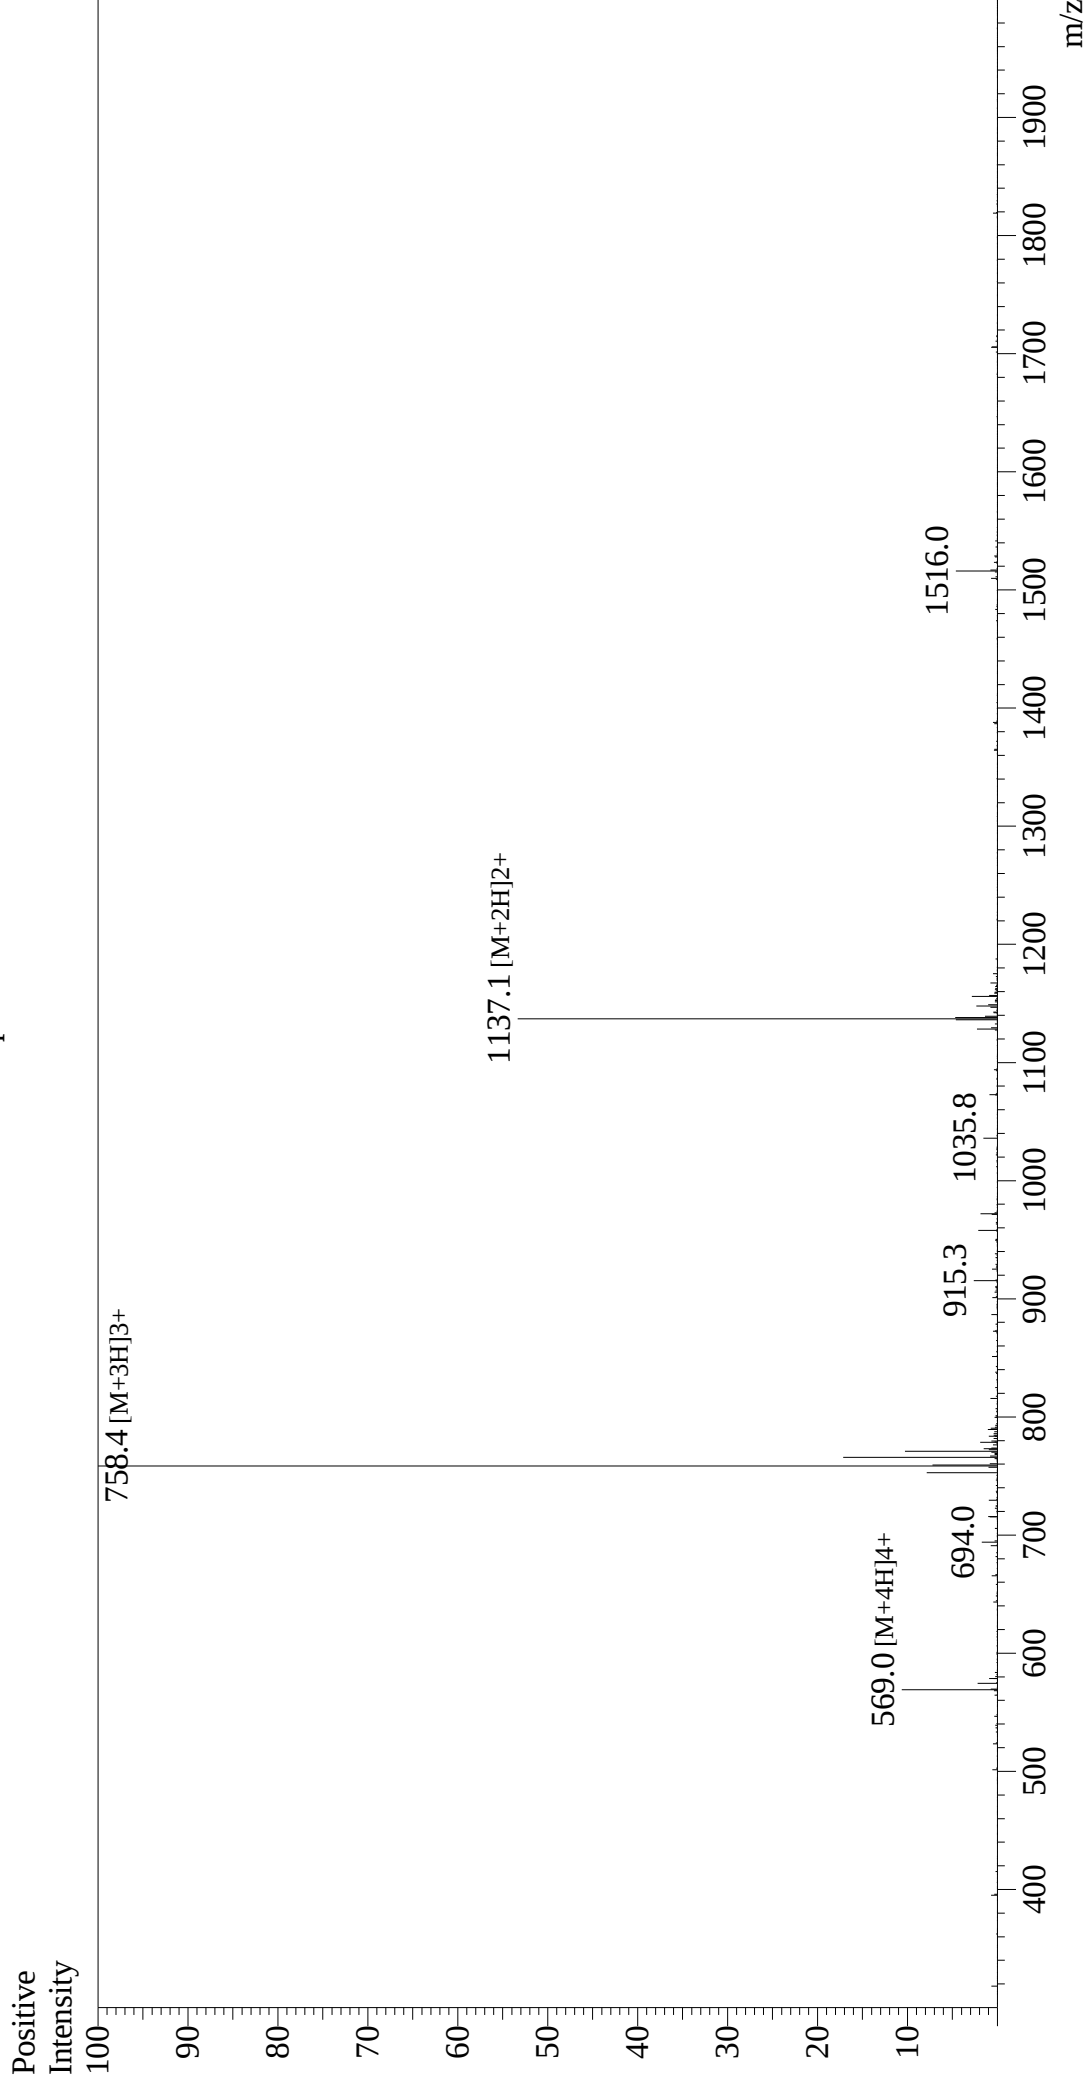

Sample Information

Month-Day Processed : 11/06/25
Time Processed : 9:17:14
Injection Volume : 0.3
Sample Name : Flagelin22
Cat No. : RP19986
Lot No. : E8239325K
Theoretical MW : 2272.50
Observed MW : 2272.2

Interface

Interface : ESI
Nebulizing Gas Flow : 1.5L/min
CDL Temp : 250
Block Temp : 200

Equipment

Equipment : ZJ21010035
Interface Bias : +4.5 kV
Drying Gas Flow : 5 L/min
T.Flow : 0.2 ml/min
B.conc : 50%H₂O/50%MeOH