


Mass Spectrum

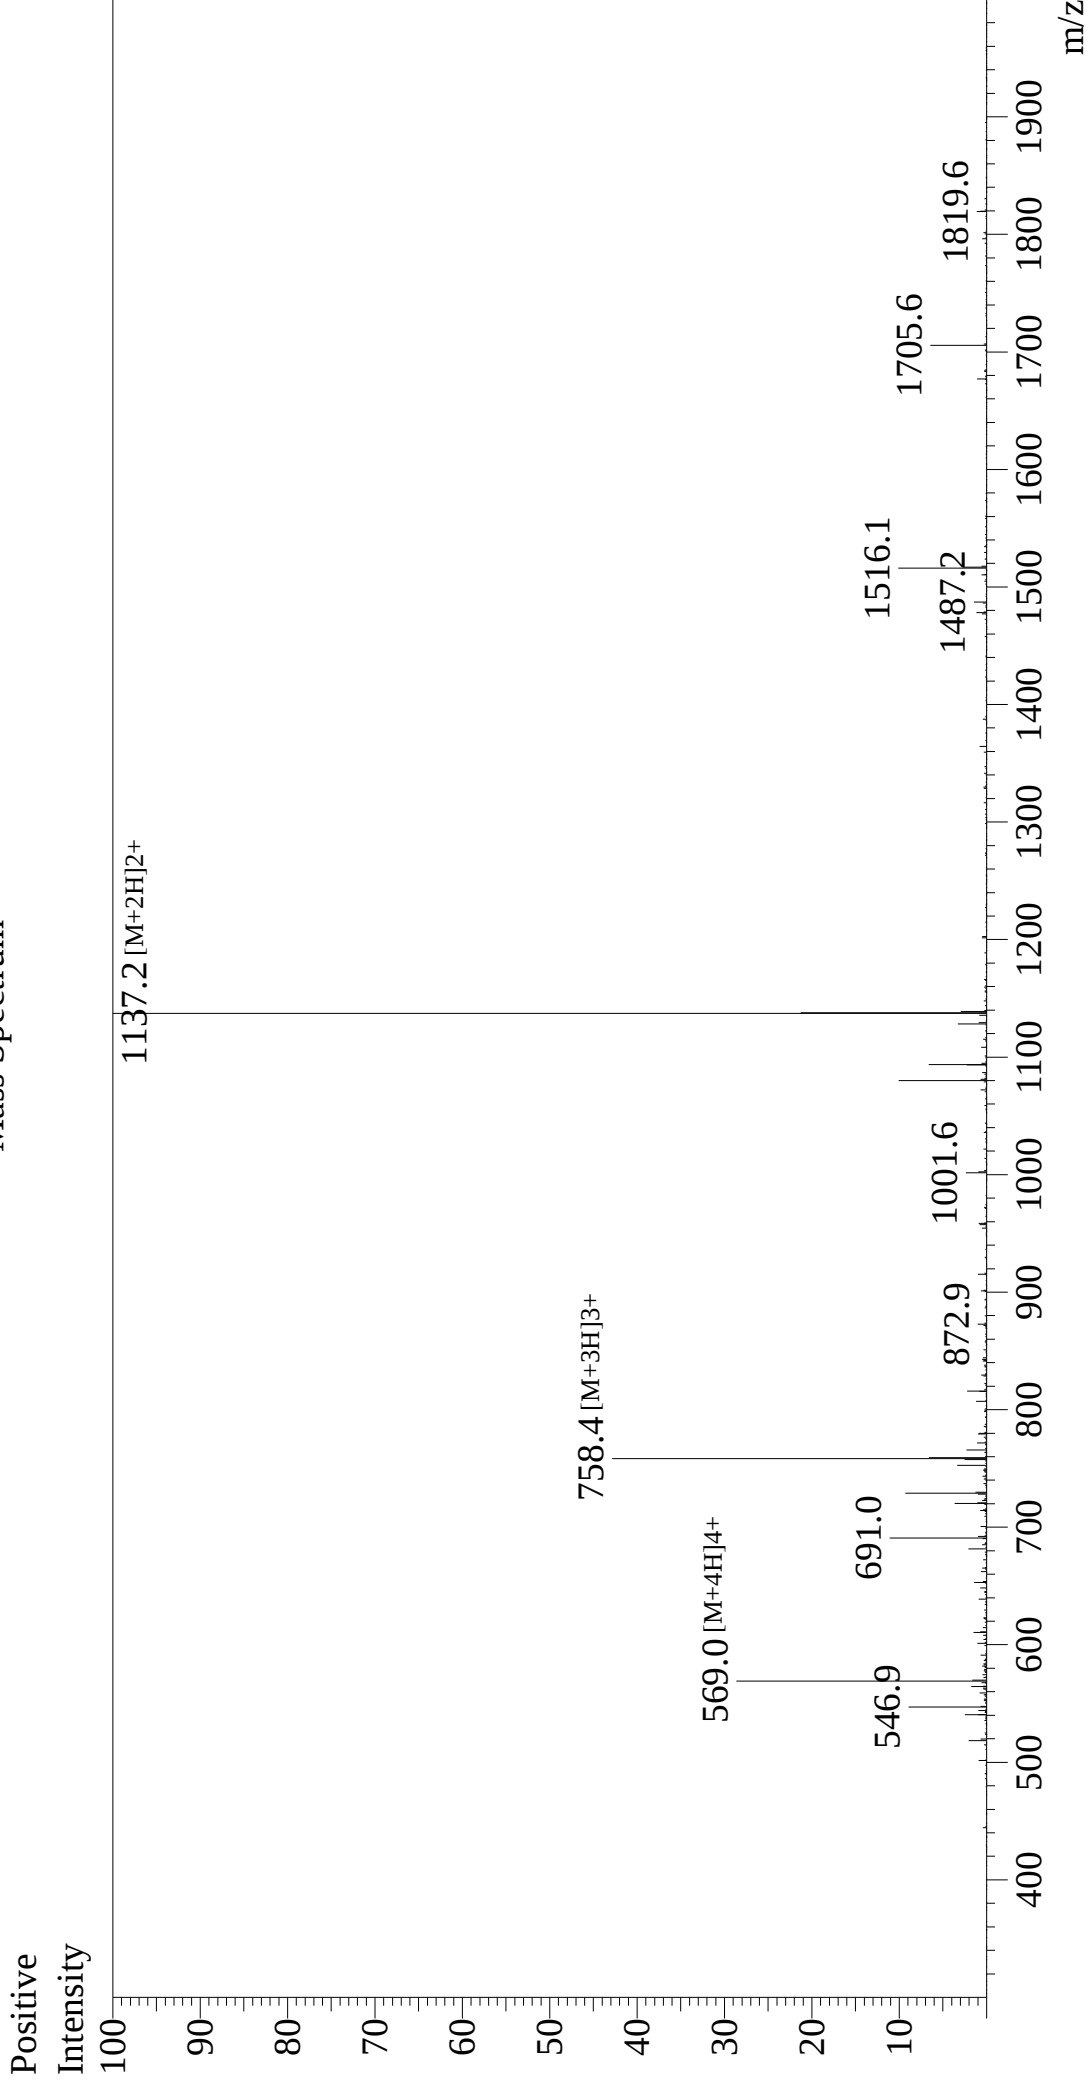

Sample Information

Month-Day Processed : 05/26/26
Time Processed : 8:59:24
Injection Volume : 0.5
Sample Name : Flagelin22
Cat No. : RP19986
Lot No. : E9604826E

Theoretical MW: 2272.51
Observed MW : 2272.4

Interface

Interface : ESI
Nebulizing Gas Flow : 1.5L/min
CDL Temp : 250
Block Temp : 200

Equipment

Equipment : ZJ21010035
Interface Bias : +4.5 kV
Drying Gas Flow : 5 L/min
T.Flow : 0.2 ml/min
B.conc : 50%H2O/50%MeOH